
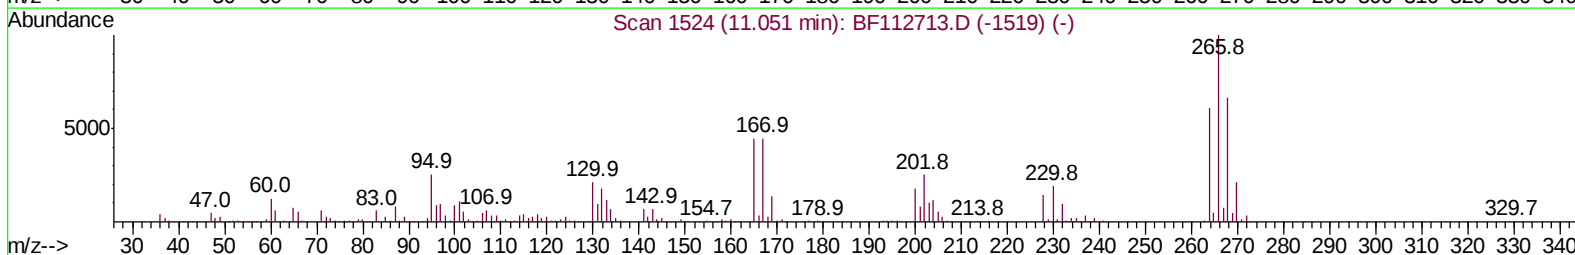
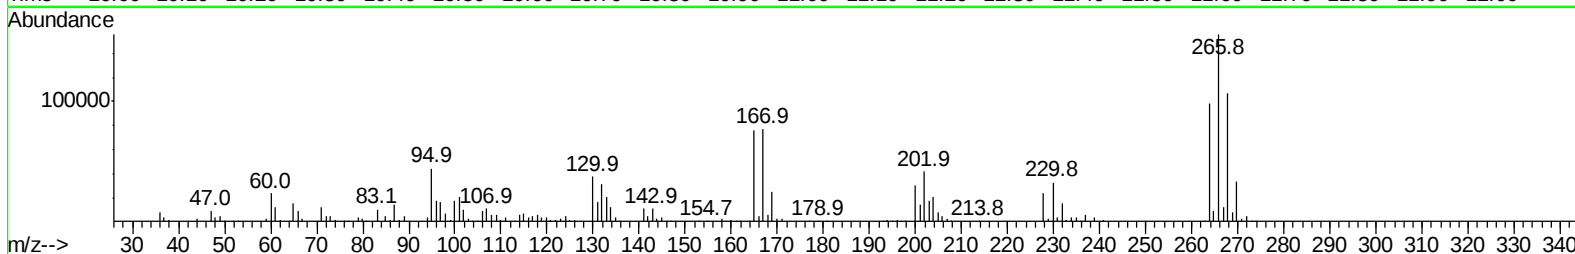


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022719\
Data File : BF112718.D
Acq On : 27 Feb 2019 14:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:02:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 27 16:08:50 2019
Response via : Initial Calibration

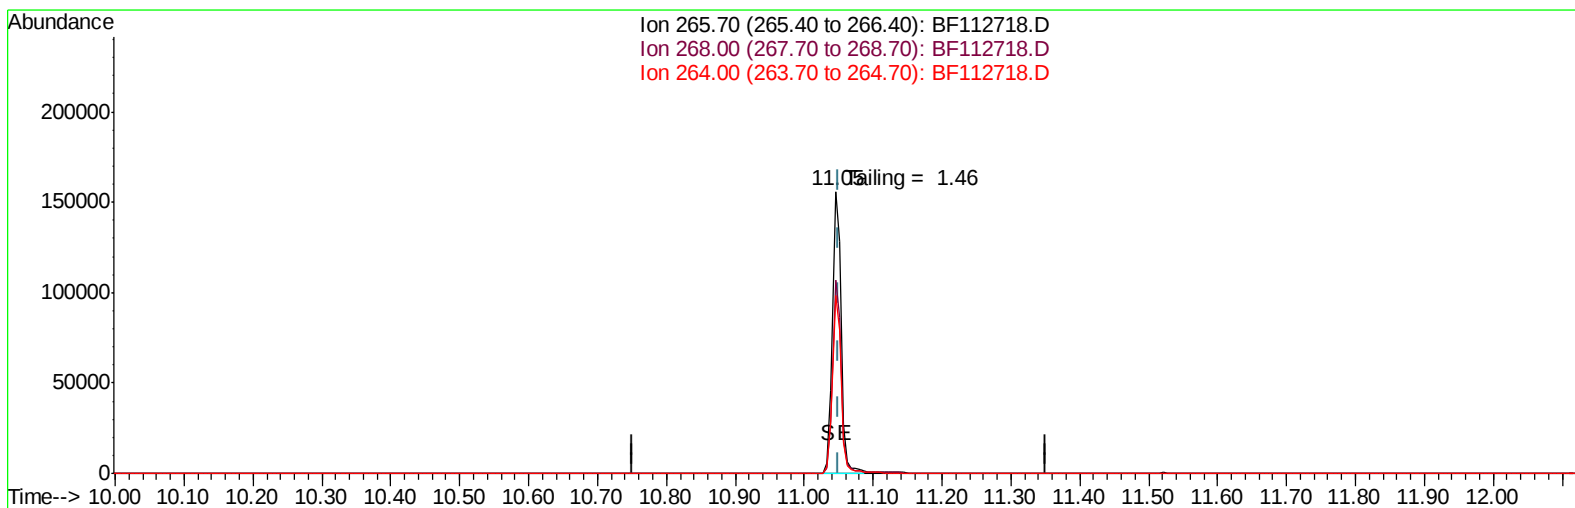

TIC: BF112718.D

(70) Pentachlorophenol (C)




11.045min (-0.006) 0.00ng

response 135380

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	68.57
264.00	61.10	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022719\
Data File : BF112718.D
Acq On : 27 Feb 2019 14:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:02:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 27 16:08:50 2019
Response via : Initial Calibration

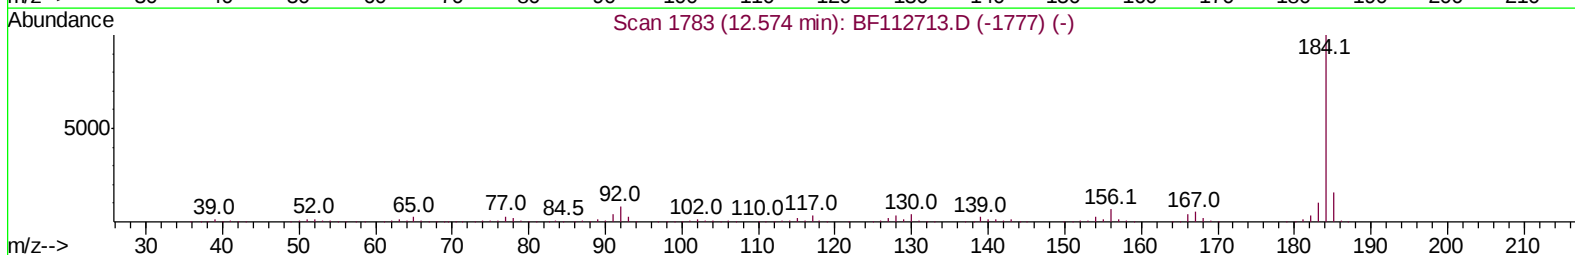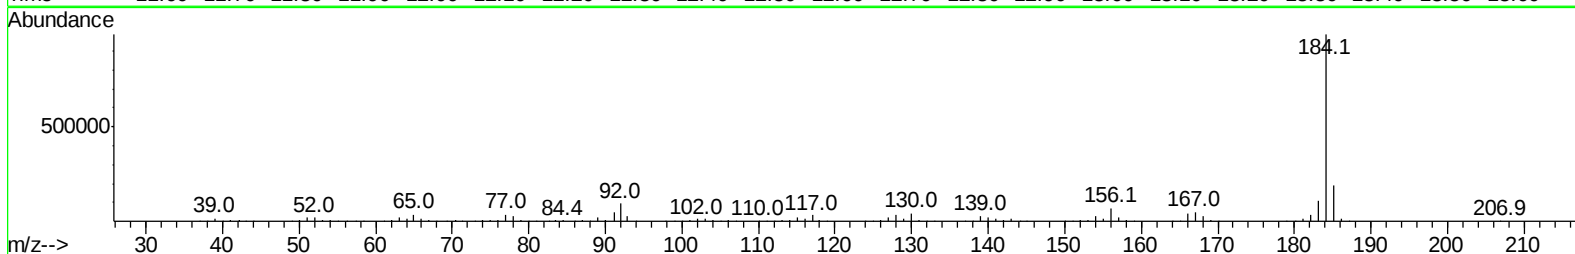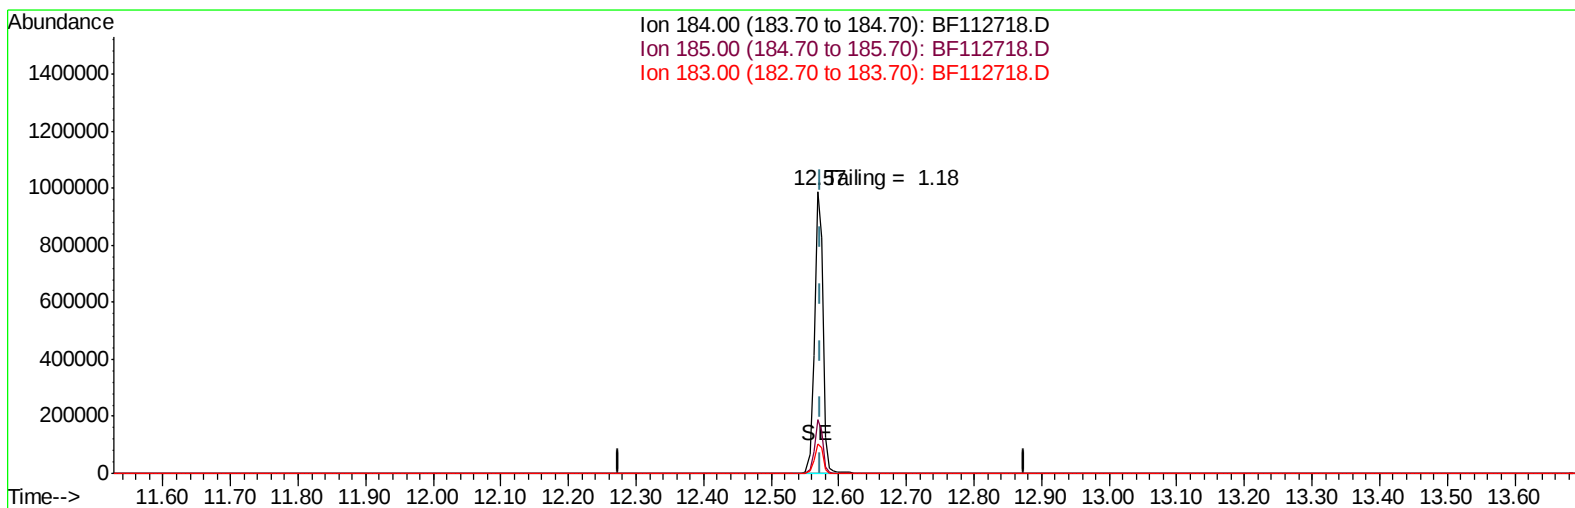

TIC: BF112718.D

(77) Benzidine

12.568min (-0.006) 0.00ng

response 873695

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	19.13#
183.00	10.70	10.68
0.00	0.00	0.00