

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022719\
 Data File : BF112748.D
 Acq On : 28 Feb 2019 5:30
 Operator : JU/SJ
 Sample : K1611-03 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HP-627

Quant Time: Feb 28 06:48:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 27 16:08:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	178718	20.00	ng	0.00
21) Naphthalene-d8	8.02	136	638719	20.00	ng	0.00
39) Acenaphthene-d10	9.77	164	283426	20.00	ng	0.00
64) Phenanthrene-d10	11.25	188	577898	20.00	ng	0.00
76) Chrysene-d12	13.87	240	444546	20.00	ng	0.00
87) Perylene-d12	15.28	264	303149	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	123554	10.75	ng	0.00
7) Phenol-d6	6.36	99	124208	8.61	ng	0.00
23) Nitrobenzene-d5	7.30	82	203695	19.08	ng	0.00
42) 2,4,6-Tribromophenol	10.55	330	65834	21.88	ng	0.00
45) 2-Fluorobiphenyl	9.10	172	420603	14.54	ng	0.00
79) Terphenyl-d14	12.83	244	473147	20.63	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022719\
Data File : BF112748.D
Acq On : 28 Feb 2019 5:30
Operator : JU/SJ
Sample : K1611-03 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HP-627

Quant Time: Feb 28 06:48:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 27 16:08:50 2019
Response via : Initial Calibration

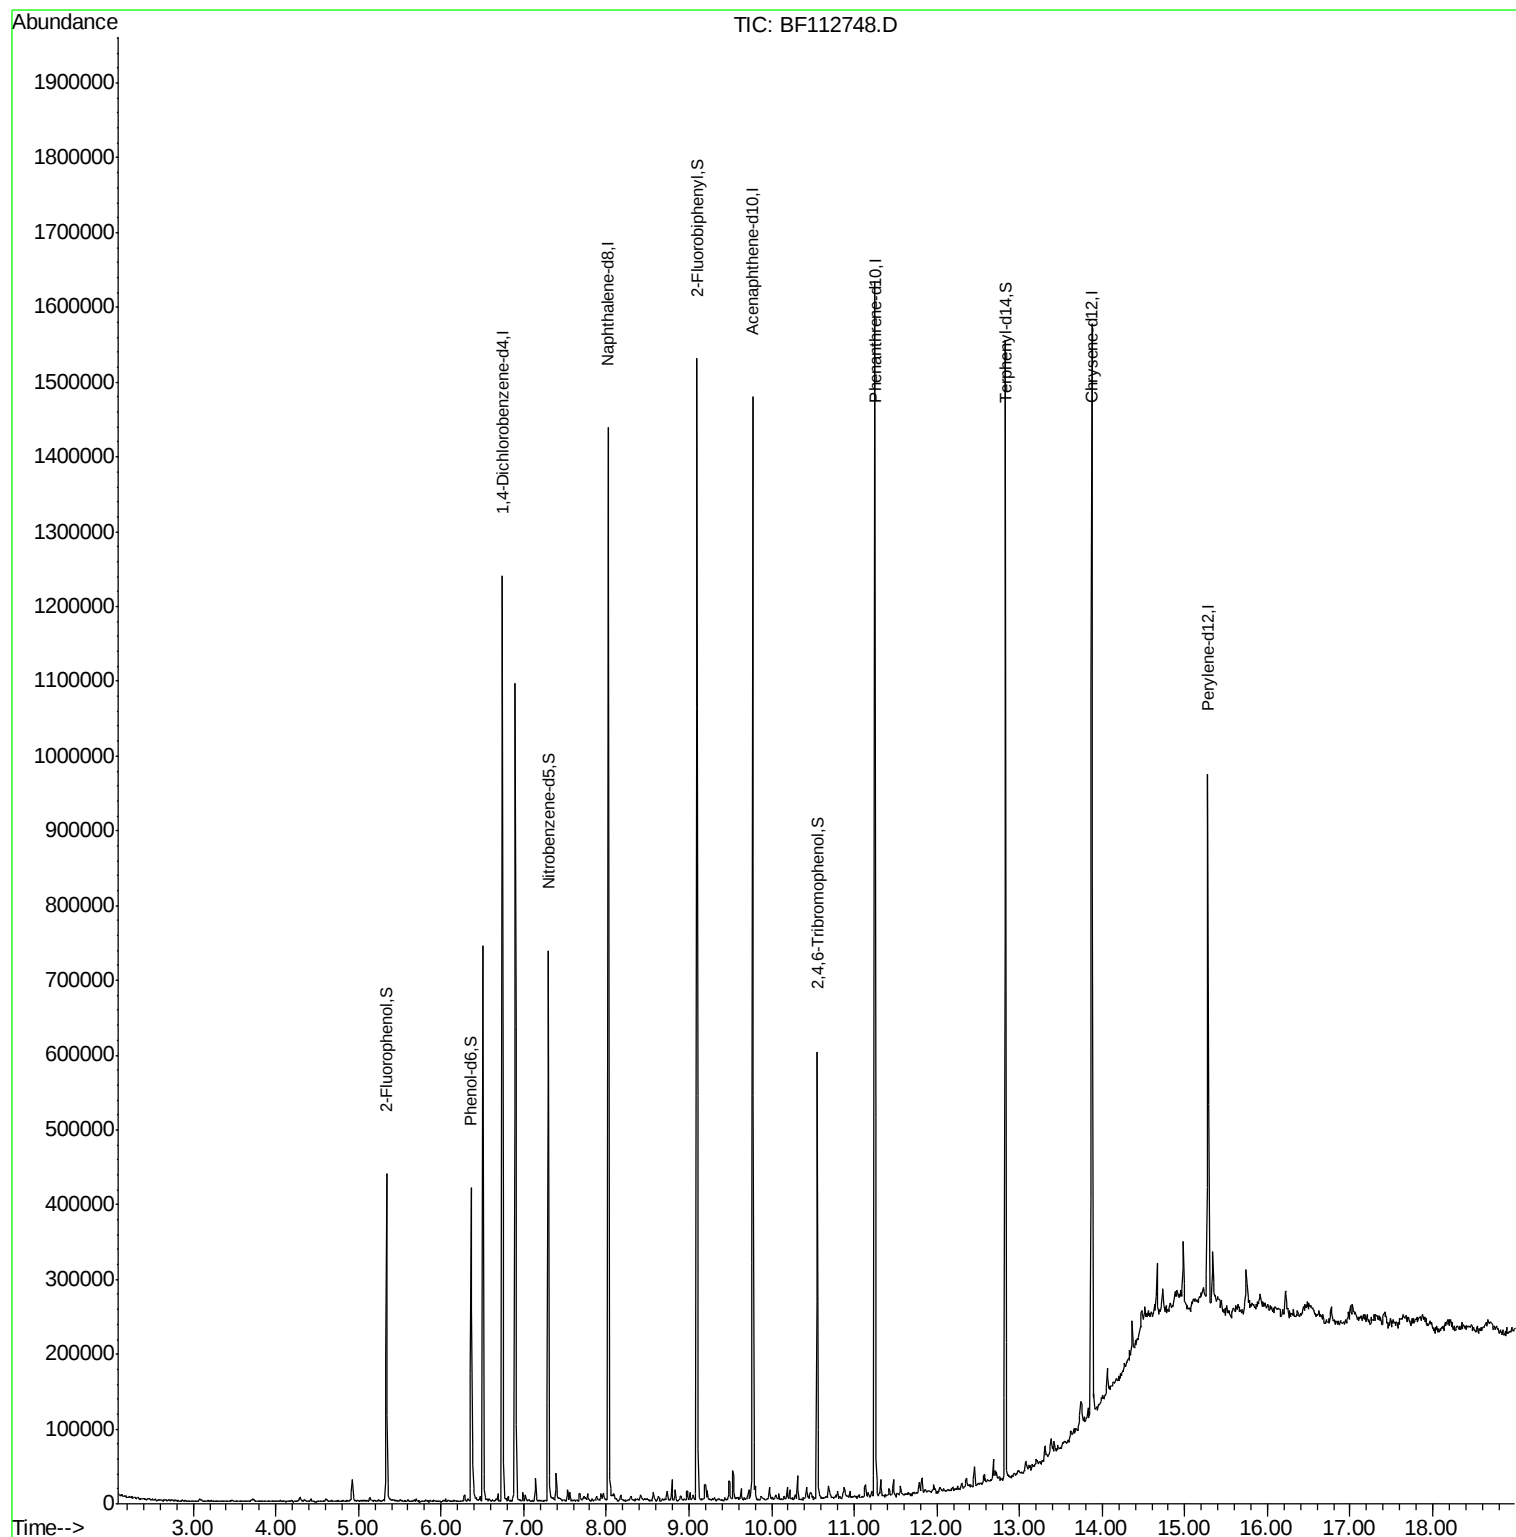

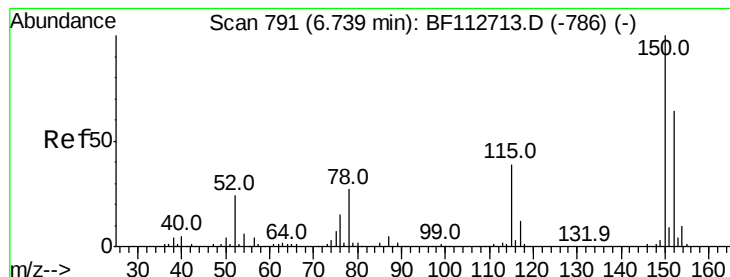


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 792
Delta R.T. 0.01 min
Lab File: BF112748.D
Acq: 28 Feb 2019 5:30

Instrument :
BNA_F
ClientSampleId :
HP-627

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.6	124.2	186.2
115	59.7	48.2	72.4



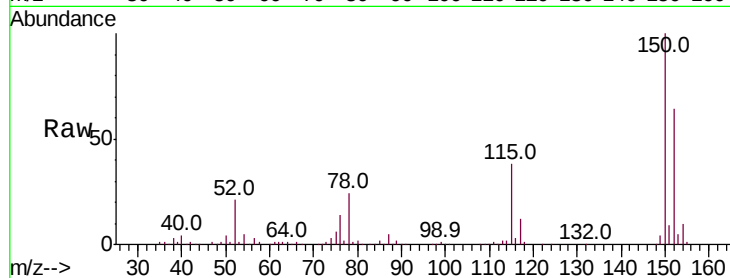


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

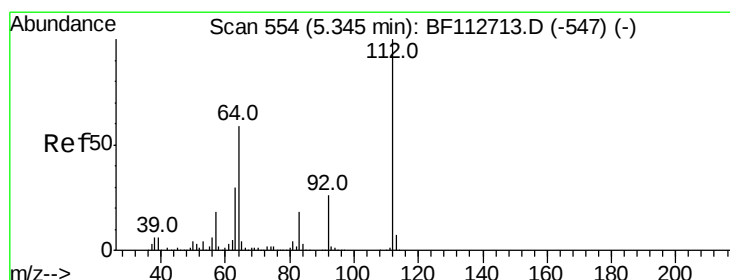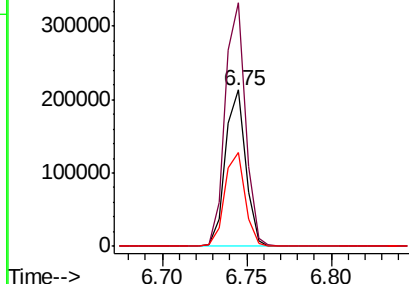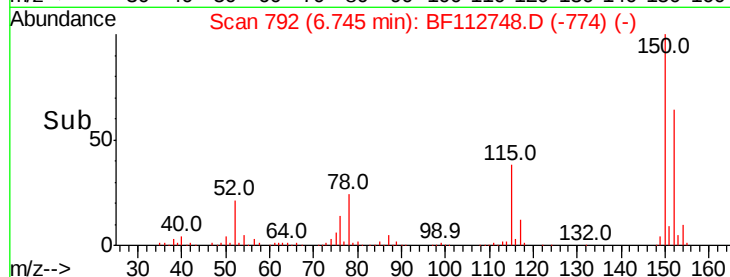

#5

2-Fluorophenol
Concen: 10.754 ng
RT: 5.34 min Scan# 553
Delta R.T. -0.01 min
Lab File: BF112748.D
Acq: 28 Feb 2019 5:30

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.6	47.6	71.4
63	28.8	24.4	36.6


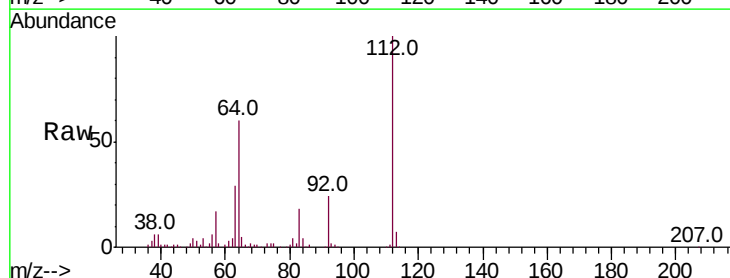



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

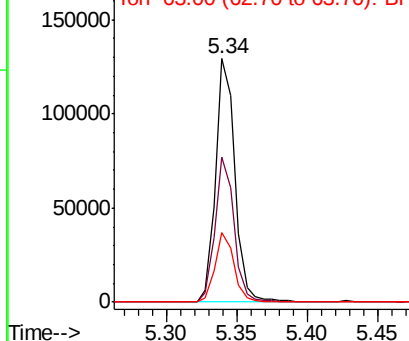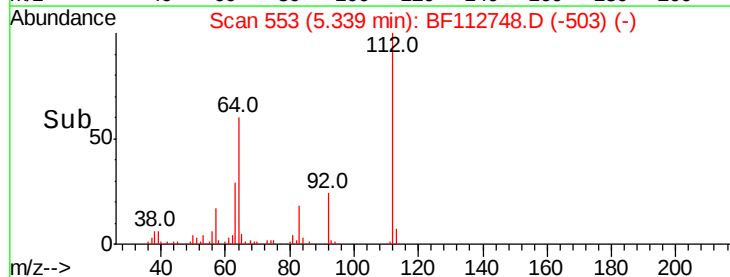

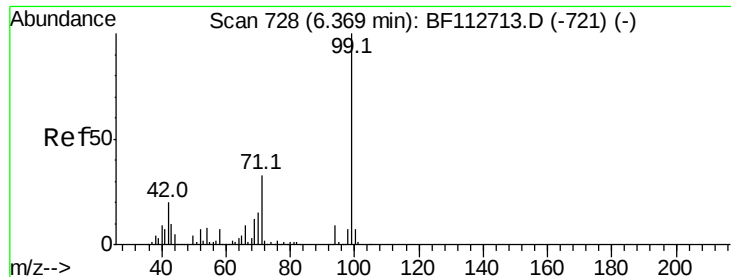

#7

Phenol-d6

Concen: 8.606 ng

RT: 6.36 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF112748.D

Acq: 28 Feb 2019 5:30

Instrument :

BNA_F

ClientSampleId :

HP-627





Tot Ion: 99 Resp: 124208

Ion Ratio Lower Upper

99 100

42 17.5 16.3 24.5

71 30.1 26.2 39.4

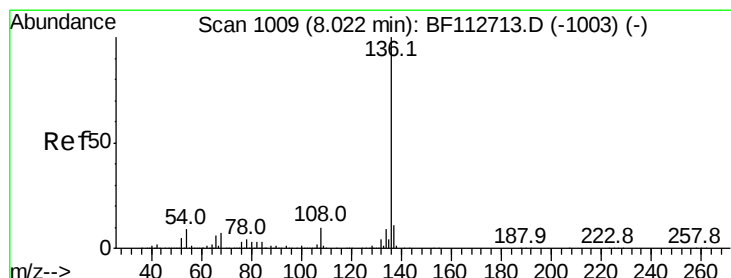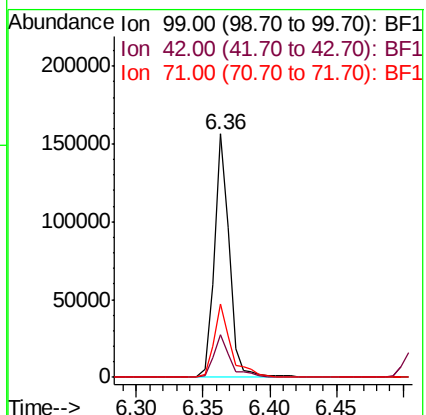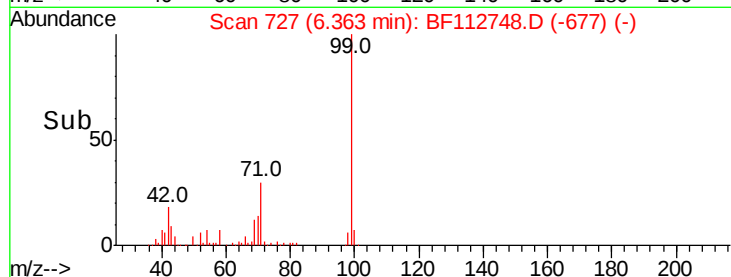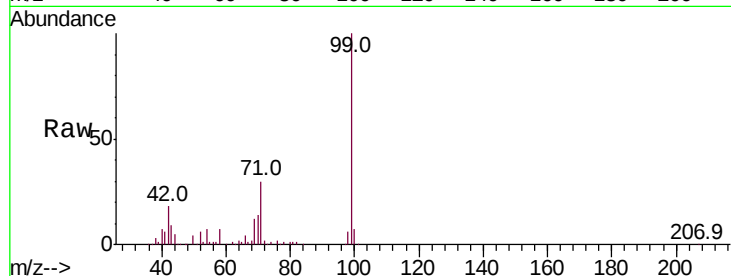

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 1009

Delta R.T. -0.00 min

Lab File: BF112748.D

Acq: 28 Feb 2019 5:30

Tgt Ion: 136 Resp: 638719




Ion Ratio Lower Upper


136 100

137 11.3 8.9 13.3

54 9.0 7.3 10.9

68 6.6 5.4 8.2


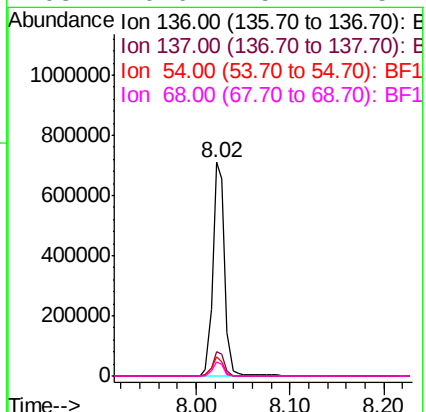
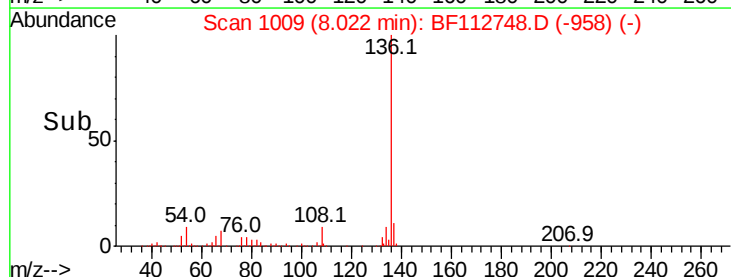
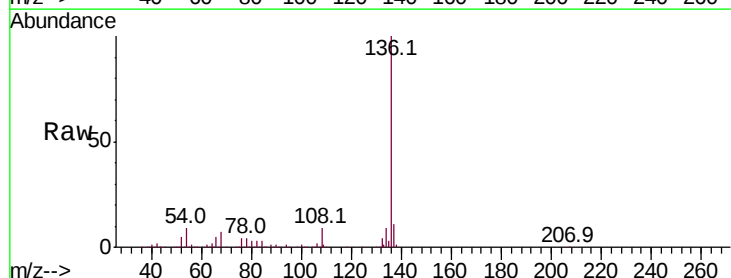


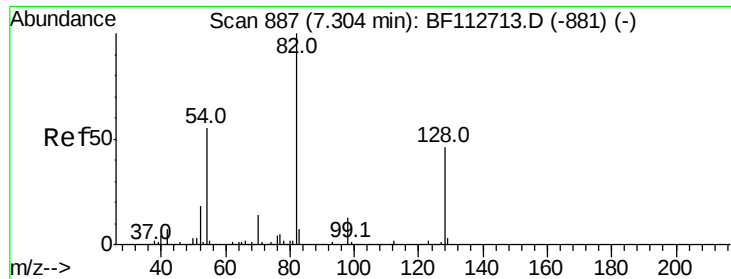

#23
 Nitrobenzene-d5
 Concen: 19.083 ng
 RT: 7.30 min Scan# 886
 Delta R.T. -0.01 min
 Lab File: BF112748.D
 Acq: 28 Feb 2019 5:30




Instrument :
 BNA_F
 ClientSampleId :
 HP-627


Tot Ion	82	Resp	203695
Ion Ratio	Lower	Upper	
82	100		
128	46.3	36.3	54.5
54	51.9	43.7	65.5

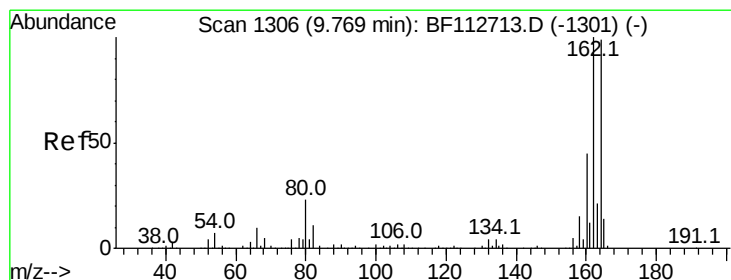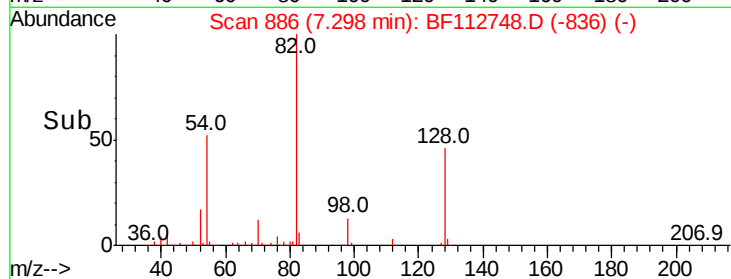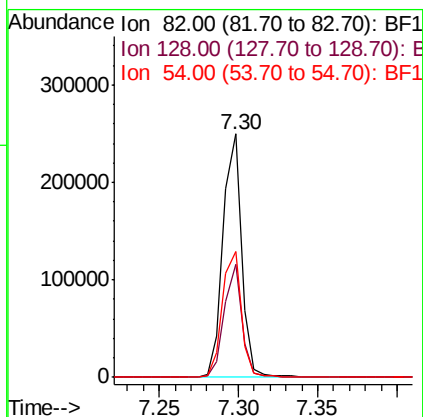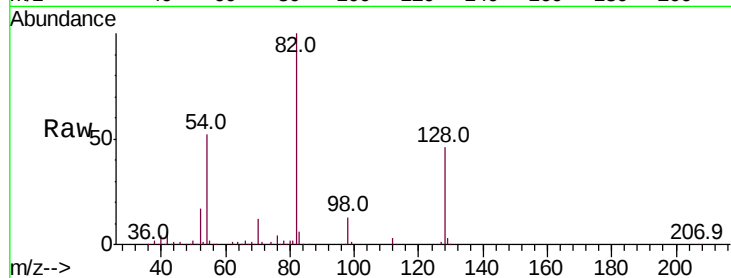

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.77 min Scan# 1307
 Delta R.T. 0.01 min
 Lab File: BF112748.D
 Acq: 28 Feb 2019 5:30

Tgt Ion	164	Resp	283426
Ion Ratio	Lower	Upper	
164	100		
162	102.5	80.6	120.8
160	46.5	36.0	54.0

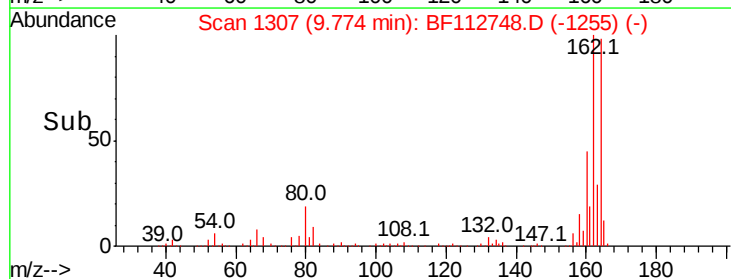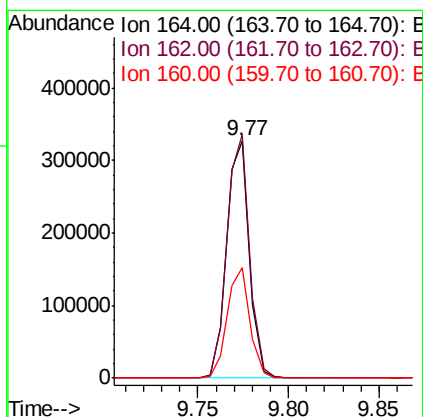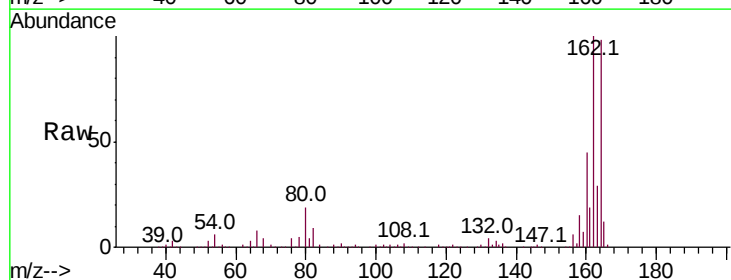

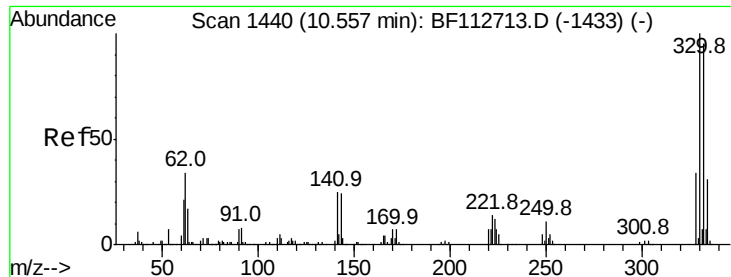

#42

2,4,6-Tribromophenol

Concen: 21.880 ng

RT: 10.55 min Scan# 1439

Delta R.T. -0.01 min

Lab File: BF112748.D

Acq: 28 Feb 2019 5:30

Instrument :

BNA_F

ClientSampled :

HP-627


Tot Ion:330 Resp: 65834

Ion Ratio Lower Upper

330 100

332 97.9 76.2 114.4




141 31.9 27.0 40.6

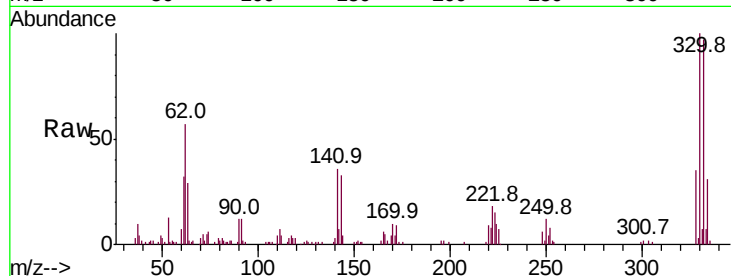

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

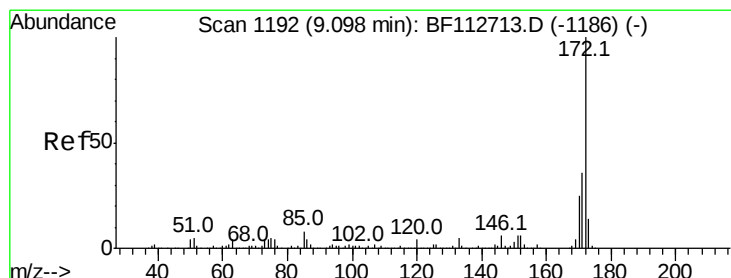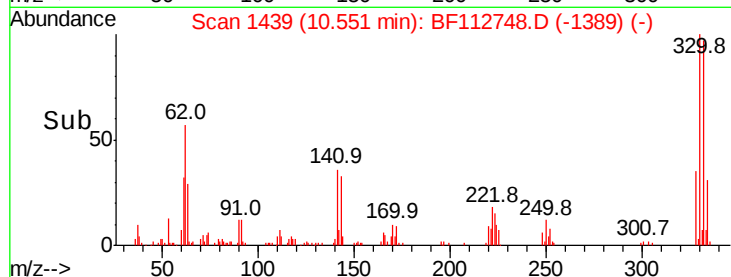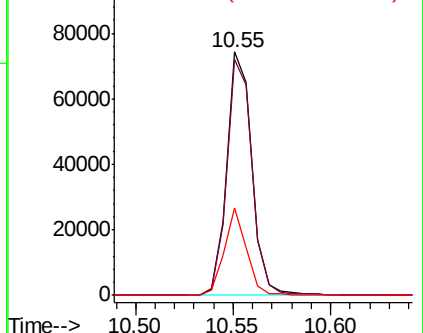

#45

2-Fluorobiphenyl

Concen: 14.537 ng

RT: 9.10 min Scan# 1192

Delta R.T. -0.00 min

Lab File: BF112748.D

Acq: 28 Feb 2019 5:30


Tgt Ion:172 Resp: 420603

Ion Ratio Lower Upper

172 100

171 34.3 29.0 43.4



170 23.4 20.0 30.0

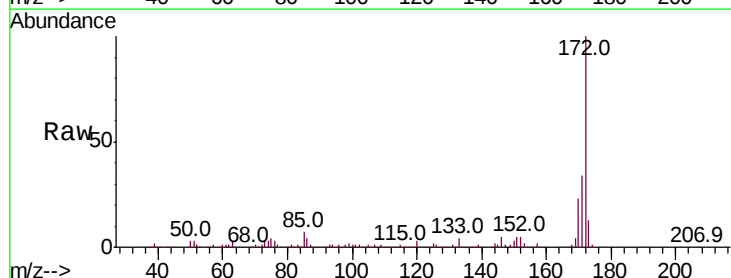


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

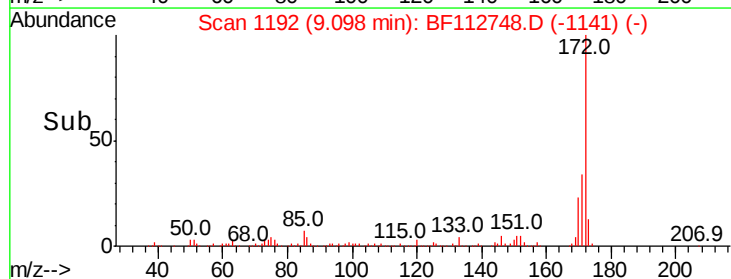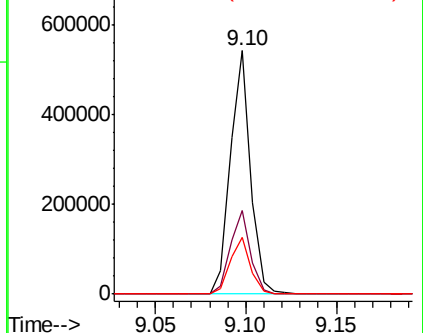

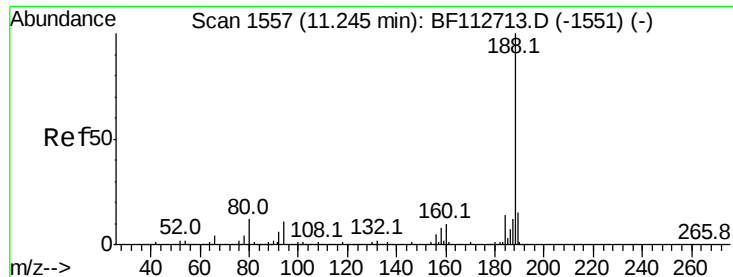

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.25 min Scan# 1558

Delta R.T. 0.01 min

Lab File: BF112748.D

Acq: 28 Feb 2019 5:30

Instrument :

BNA_F

ClientSampleId :

HP-627


Tot Ion:188 Resp: 577898

Ion Ratio Lower Upper

188 100

94 9.7 9.0 13.4


80 10.0 9.2 13.8

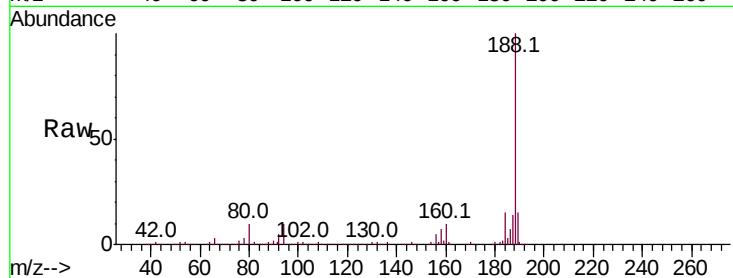



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

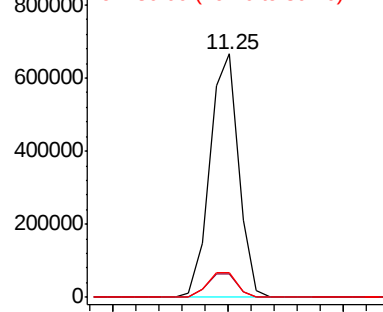

Time-->

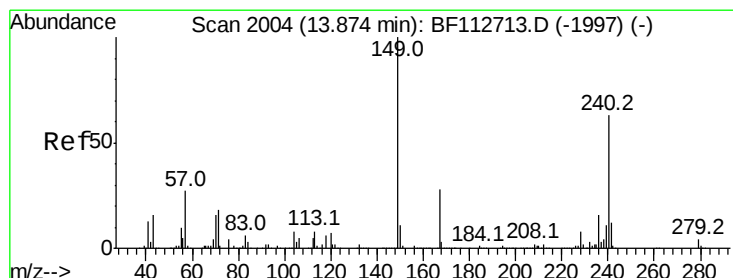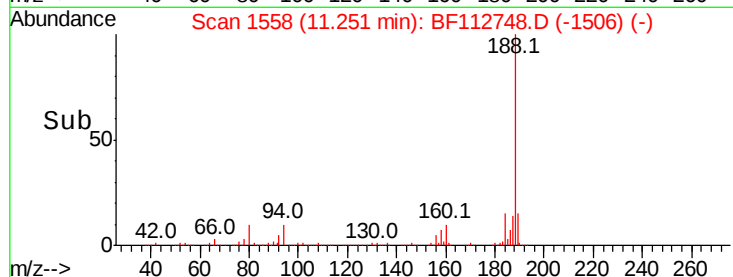

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.87 min Scan# 2004

Delta R.T. -0.00 min

Lab File: BF112748.D

Acq: 28 Feb 2019 5:30


Tgt Ion:240 Resp: 444546

Ion Ratio Lower Upper

240 100

120 12.3 8.9 13.3


236 25.6 20.7 31.1

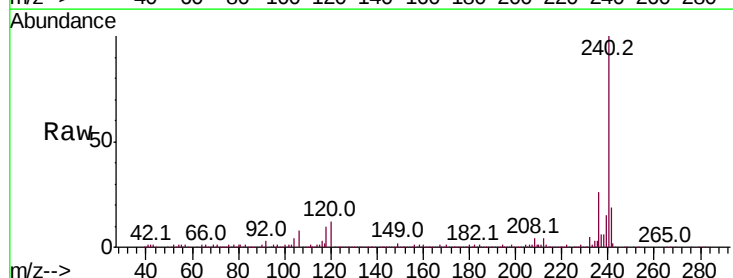


Abundance Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

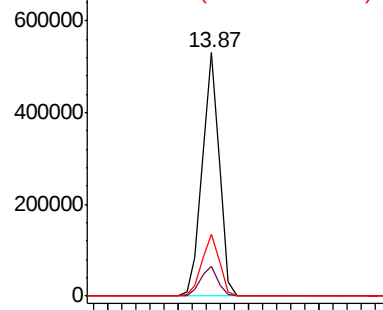

Time-->

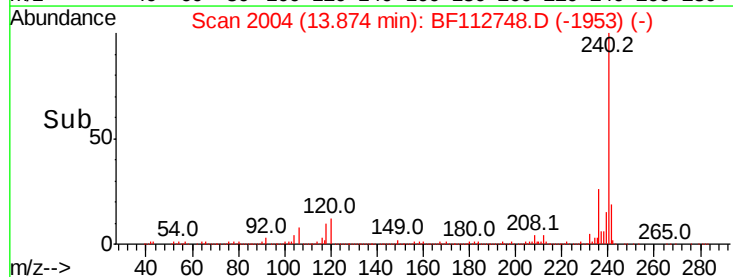

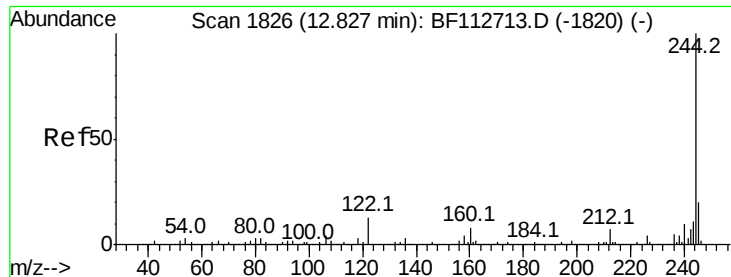

#79

Terphenyl-d14

Concen: 20.632 ng

RT: 12.83 min Scan# 1826

Delta R.T. -0.00 min

Lab File: BF112748.D

Acq: 28 Feb 2019 5:30

Instrument :

BNA_F

ClientSampleId :

HP-627


Tot Ion:244 Resp: 473147

Ion Ratio Lower Upper

244 100

212 6.7 5.6 8.4




122 13.0 10.5 15.7

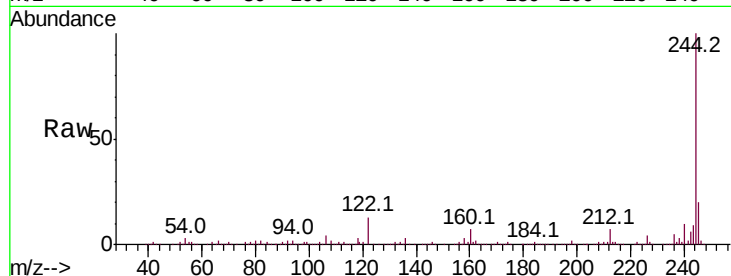

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

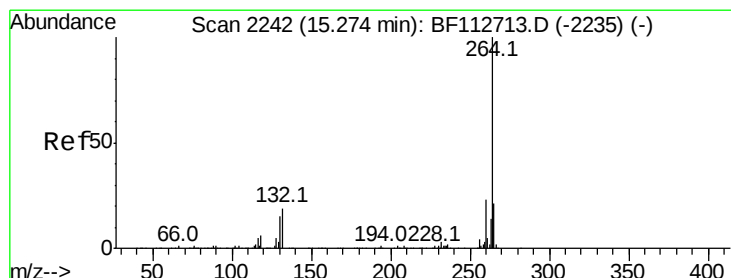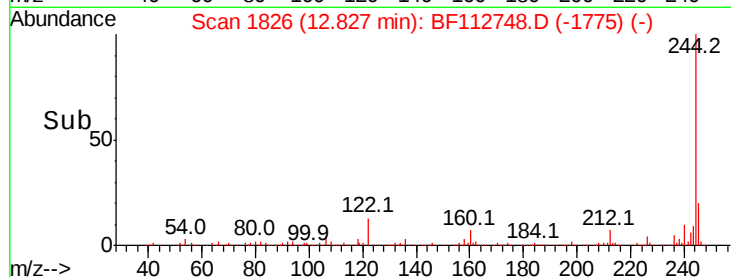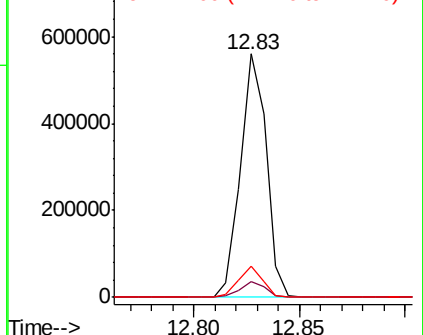

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.28 min Scan# 2243

Delta R.T. 0.01 min

Lab File: BF112748.D

Acq: 28 Feb 2019 5:30


Tgt Ion:264 Resp: 303149

Ion Ratio Lower Upper

264 100

260 23.4 18.7 28.1

265 21.9 17.2 25.8

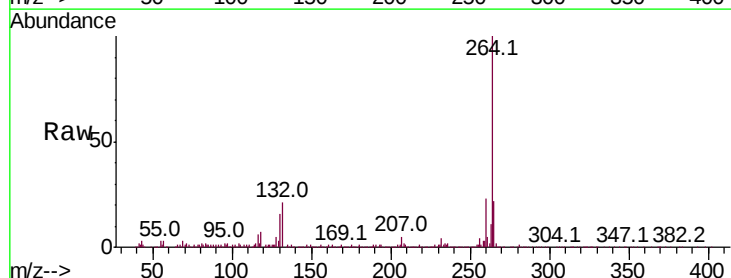

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

