

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022719\
 Data File : BF112725.D
 Acq On : 27 Feb 2019 18:03
 Operator : JU/SJ
 Sample : K1627-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-02-(2-5)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	178	180	191	rBV5	20159	55056	1.21%	0.114%
2	5.346	549	554	557	rBV	4165255	4349694	95.89%	9.030%
3	6.369	722	728	731	rBV	4314628	4536327	100.00%	9.417%
4	6.504	747	751	755	rVB	4385858	4401415	97.03%	9.137%
5	6.740	787	791	794	rBV	1651566	1273756	28.08%	2.644%
6	6.810	799	803	809	rBV	86622	75579	1.67%	0.157%
7	6.898	813	818	821	rVV	3864221	3404129	75.04%	7.067%
8	7.298	881	886	889	rBV	3083371	2772976	61.13%	5.757%
9	8.016	1004	1008	1011	rBV	1847129	1595406	35.17%	3.312%
10	9.092	1187	1191	1195	rBV	4762045	4496975	99.13%	9.335%
11	9.375	1236	1239	1243	rVB	103764	81049	1.79%	0.168%
12	9.486	1254	1258	1260	rBV	302556	252924	5.58%	0.525%
13	9.769	1302	1306	1309	rBV	1726904	1584257	34.92%	3.289%
14	10.045	1349	1353	1355	rBV	55233	53663	1.18%	0.111%
15	10.545	1434	1438	1442	rBV	2749718	2456370	54.15%	5.099%
16	10.698	1460	1464	1469	rVB3	53290	66835	1.47%	0.139%
17	10.775	1474	1477	1480	rVB2	46230	46877	1.03%	0.097%
18	10.922	1498	1502	1505	rBV2	69548	68742	1.52%	0.143%
19	11.239	1552	1556	1559	rBV	1672129	1450643	31.98%	3.011%
20	11.263	1559	1560	1563	rVB	173914	98196	2.16%	0.204%
21	11.316	1563	1569	1571	rVB4	49730	61477	1.36%	0.128%
22	11.704	1632	1635	1639	rBV4	60406	81583	1.80%	0.169%
23	11.786	1644	1649	1657	rBV2	777466	875241	19.29%	1.817%
24	12.375	1747	1749	1754	rVB	49382	49642	1.09%	0.103%
25	12.445	1758	1761	1764	rBV	257460	218835	4.82%	0.454%
26	12.486	1765	1768	1772	rBV4	66746	91862	2.03%	0.191%
27	12.569	1778	1782	1792	rBV	686554	835679	18.42%	1.735%
28	12.651	1794	1796	1797	rVV	129694	99635	2.20%	0.207%
29	12.669	1797	1799	1802	rVV	208762	188667	4.16%	0.392%
30	12.698	1802	1804	1807	rVB	150253	120397	2.65%	0.250%
31	12.827	1821	1826	1829	rBV	3922677	3583633	79.00%	7.439%
32	13.727	1976	1979	1987	rVB	713829	648360	14.29%	1.346%
33	13.810	1990	1993	1996	rBV	82352	70073	1.54%	0.145%
34	13.863	1998	2002	2005	rBV	1590028	1606694	35.42%	3.335%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022719\
Data File : BF112725.D
Acq On : 27 Feb 2019 18:03
Operator : JU/SJ
Sample : K1627-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-02-(2-5)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.886	2005	2006	2009	rVB	120008	81458	1.80%	0.169%
36	13.933	2011	2014	2018	rBV	44820	48150	1.06%	0.100%
37	14.057	2032	2035	2037	rBV2	85841	75516	1.66%	0.157%
38	14.086	2037	2040	2042	rVB2	55755	49361	1.09%	0.102%
39	14.210	2058	2061	2063	rBV2	53451	52984	1.17%	0.110%
40	14.239	2064	2066	2070	rVV3	63449	78250	1.72%	0.162%
41	14.363	2084	2087	2089	rBV	182335	174098	3.84%	0.361%
42	14.392	2089	2092	2096	rVB2	223898	230096	5.07%	0.478%
43	14.657	2134	2137	2142	rVV	174100	176915	3.90%	0.367%
44	14.727	2146	2149	2153	rVV	876547	814236	17.95%	1.690%
45	14.763	2153	2155	2161	rVB3	66526	70404	1.55%	0.146%
46	14.863	2168	2172	2176	rBV2	1467002	1601214	35.30%	3.324%
47	14.974	2188	2191	2198	rVB2	214803	278813	6.15%	0.579%
48	15.121	2213	2216	2219	rBV3	130432	147542	3.25%	0.306%
49	15.210	2228	2231	2234	rBV	133113	182911	4.03%	0.380%
50	15.274	2237	2242	2245	rVV	1213435	1472310	32.46%	3.056%
51	15.333	2249	2252	2256	rVB2	160893	191944	4.23%	0.398%
52	15.480	2274	2277	2282	rBV3	80123	117369	2.59%	0.244%
53	15.739	2318	2321	2325	rBV	137667	189191	4.17%	0.393%
54	15.780	2325	2328	2337	rVB3	148627	271953	6.00%	0.565%
55	16.210	2398	2401	2405	rBV2	72706	94264	2.08%	0.196%
56	17.992	2700	2704	2711	rVB2	56137	119178	2.63%	0.247%


Sum of corrected areas: 48170804

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022719\
Data File : BF112725.D
Acq On : 27 Feb 2019 18:03
Operator : JU/SJ
Sample : K1627-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
SB-02-(2-5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

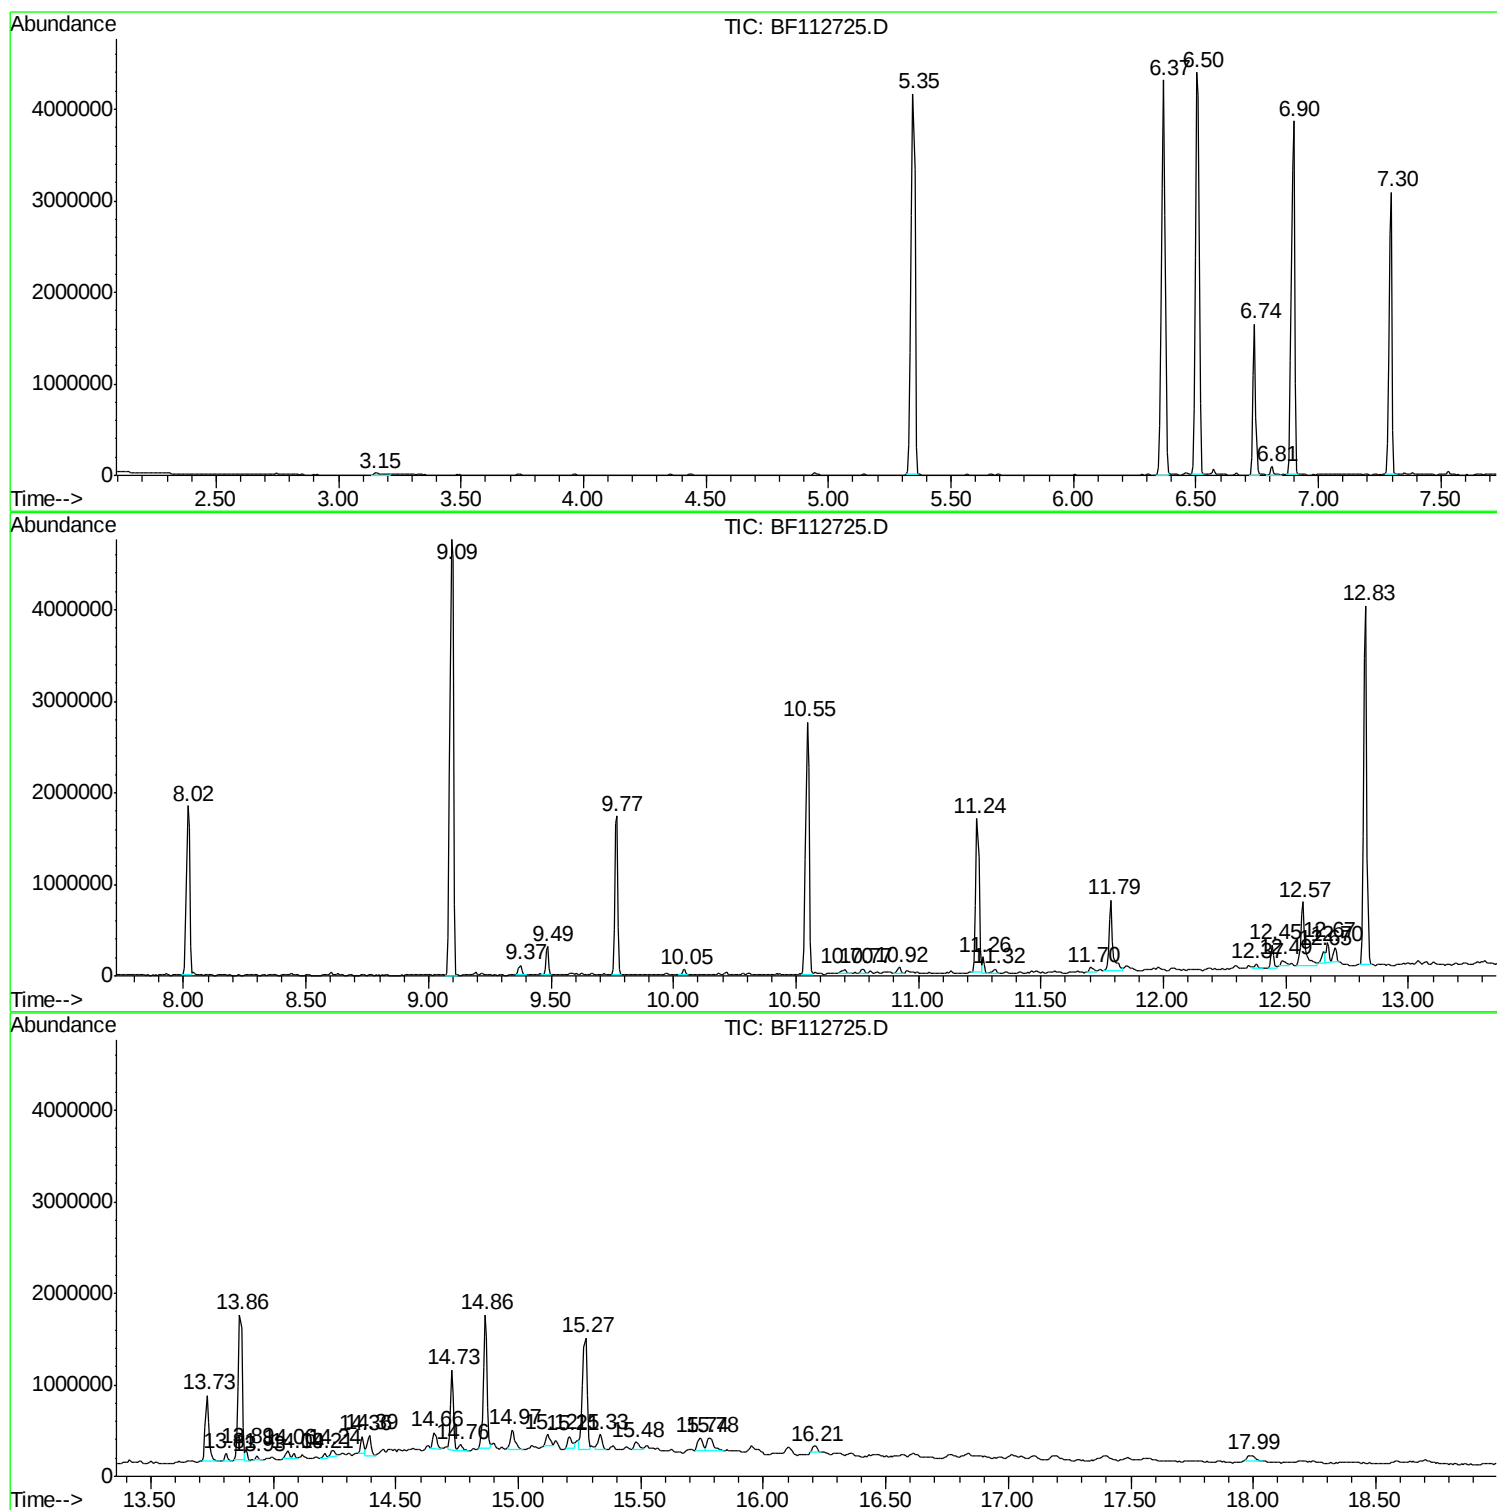

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022719\
Data_File : BF112725.D
Acq_On : 27 Feb 2019 18:033
Operator : JU/SJJ
Sample : K1627-033
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-02-(2-5)

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
