


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF022719\  
 Data File : BF112709.D  
 Acq On : 27 Feb 2019 9:09  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF022719.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Feb 27 16:08:50 2019

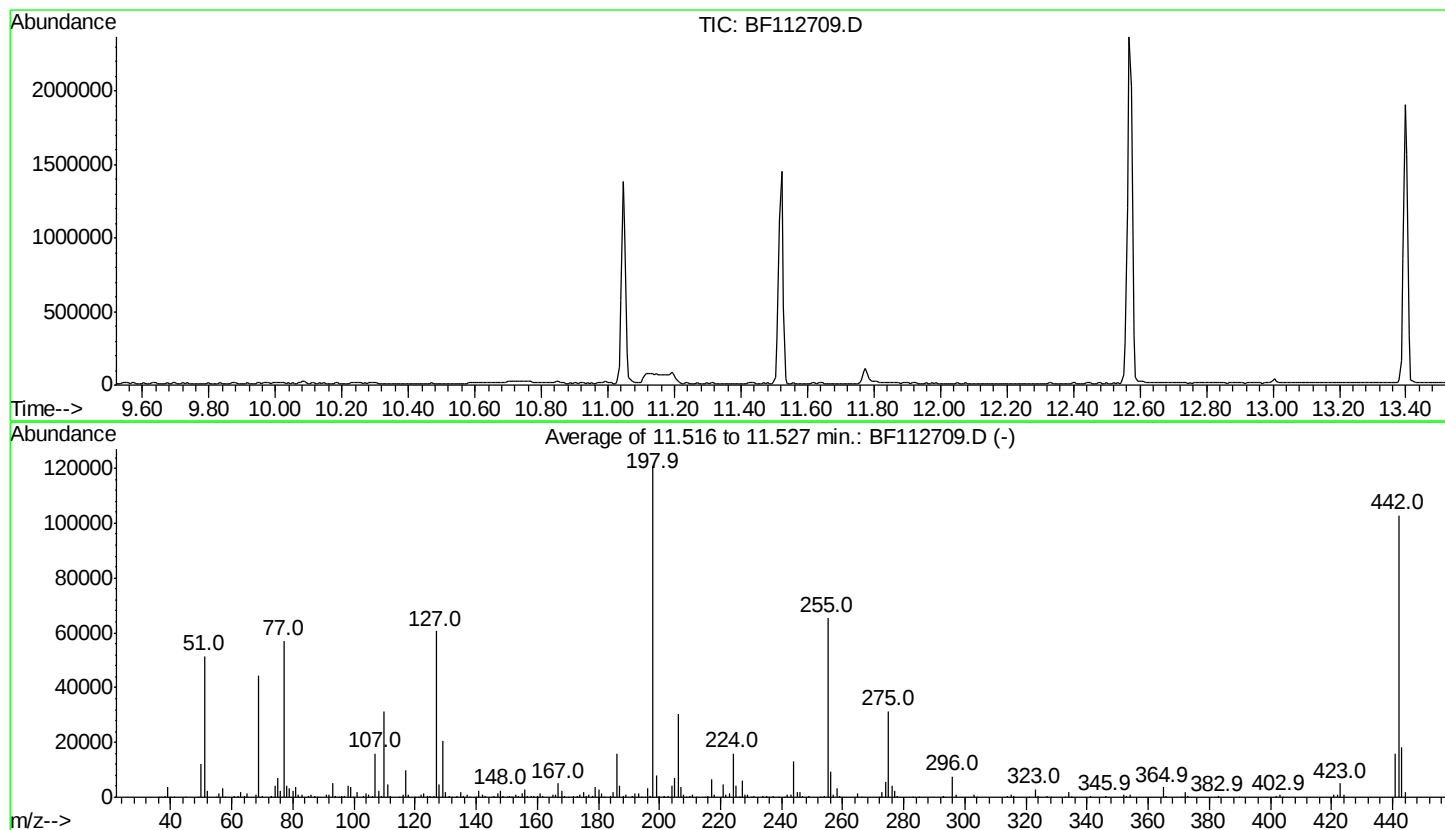

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 42.6      | 51485   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 774     | PASS             |
| 69          | 198          | 0.00         | 100          | 36.7      | 44401   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 273     | PASS             |
| 127         | 198          | 10           | 80           | 50.1      | 60568   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 434     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 120989  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 7880    | PASS             |
| 275         | 198          | 10           | 60           | 26.0      | 31434   | PASS             |
| 365         | 198          | 1            | 100          | 3.0       | 3674    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.1      | 15799   | PASS             |
| 442         | 198          | 50           | 100          | 85.0      | 102802  | PASS             |
| 443         | 442          | 15           | 24           | 17.6      | 18080   | PASS             |