


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022719\
 Data File : BF112745.D
 Acq On : 28 Feb 2019 4:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 27 16:08:50 2019

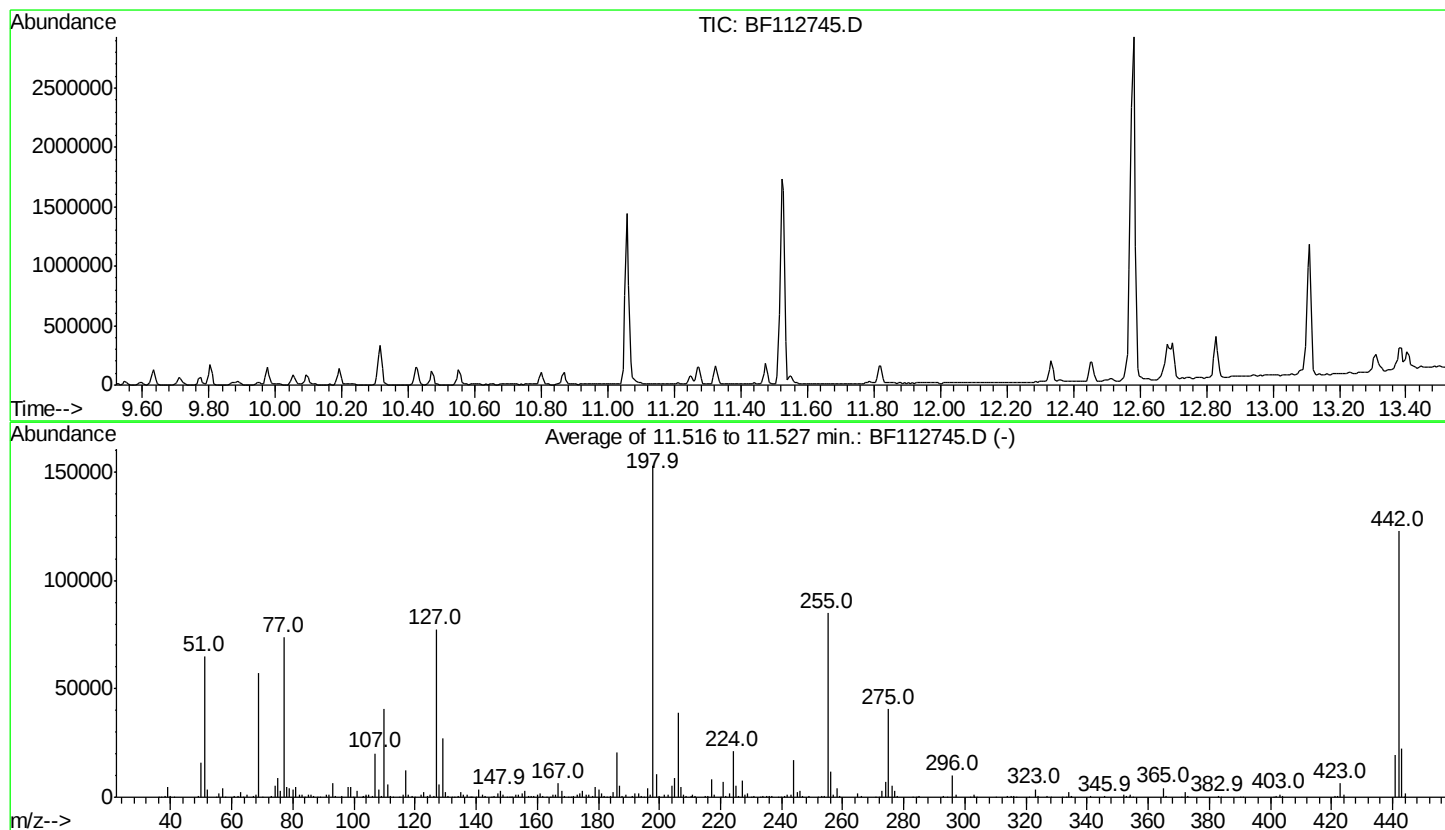

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	64834	PASS
68	69	0.00	2	1.7	961	PASS
69	198	0.00	100	37.4	57239	PASS
70	69	0.00	2	0.3	186	PASS
127	198	10	80	50.5	77306	PASS
197	198	0.00	2	0.7	1096	PASS
198	198	100	100	100.0	152960	PASS
199	198	5	9	6.9	10615	PASS
275	198	10	60	26.6	40620	PASS
365	198	1	100	2.9	4411	PASS
441	198	0.01	100	12.6	19339	PASS
442	198	50	100	80.1	122565	PASS
443	442	15	24	18.4	22513	PASS