
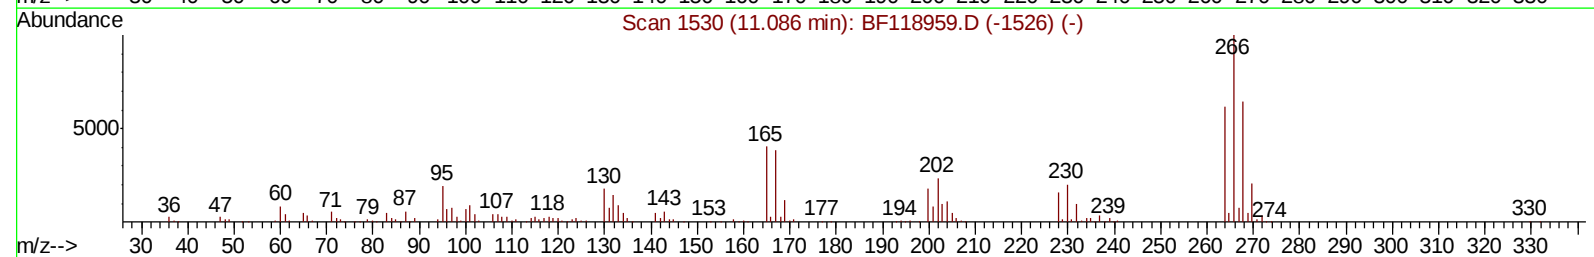
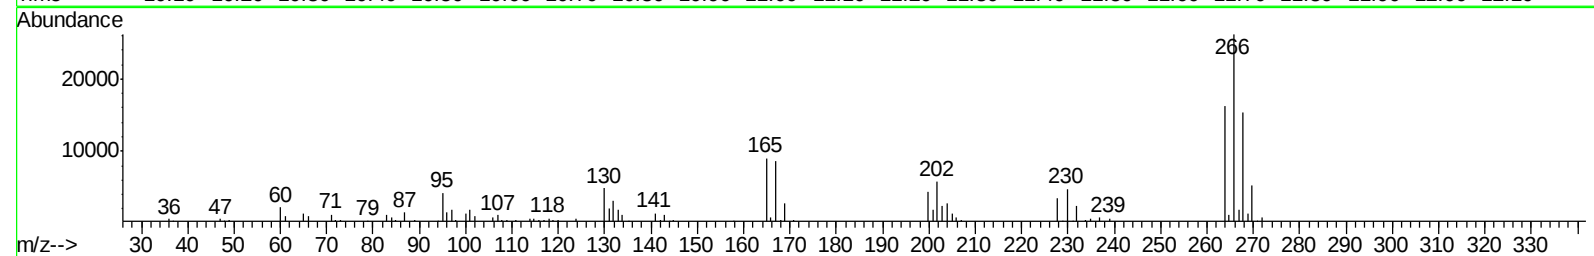


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022720\
 Data File : BF119123.D
 Acq On : 27 Feb 2020 21:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 06:56:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 26 16:03:05 2020
 Response via : Initial Calibration

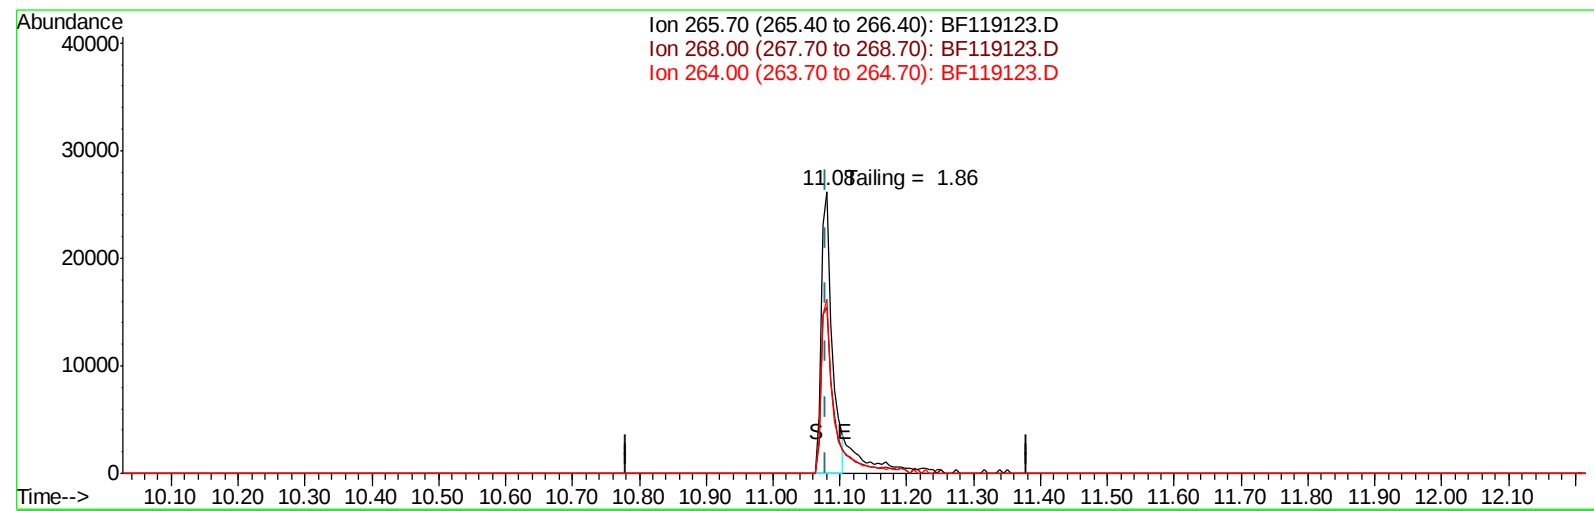

TIC: BF119123.D

(70) Pentachlorophenol (C)




11.080min (+0.000) 28080.49ng

response 36992

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	59.05
264.00	63.70	61.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022720\
Data File : BF119123.D
Acq On : 27 Feb 2020 21:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 06:56:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 26 16:03:05 2020
Response via : Initial Calibration

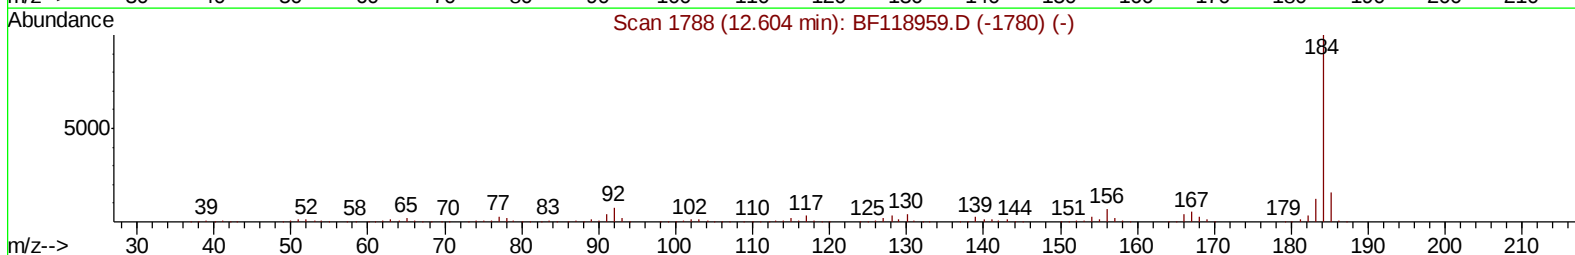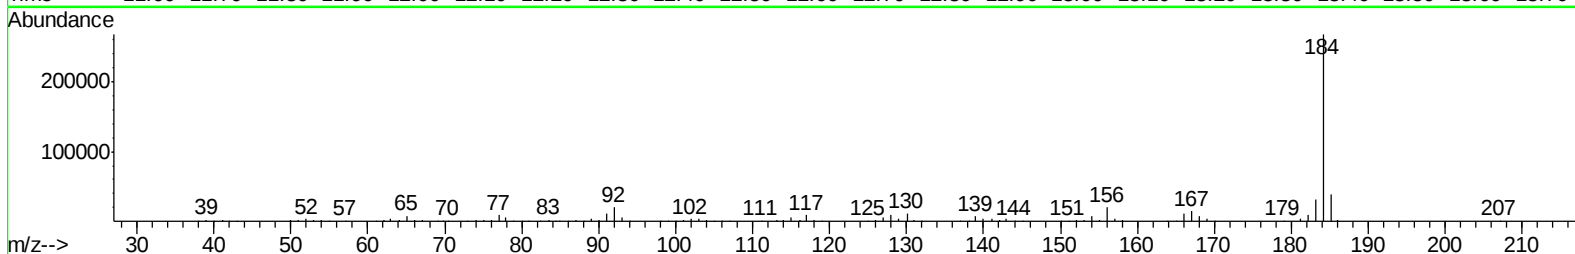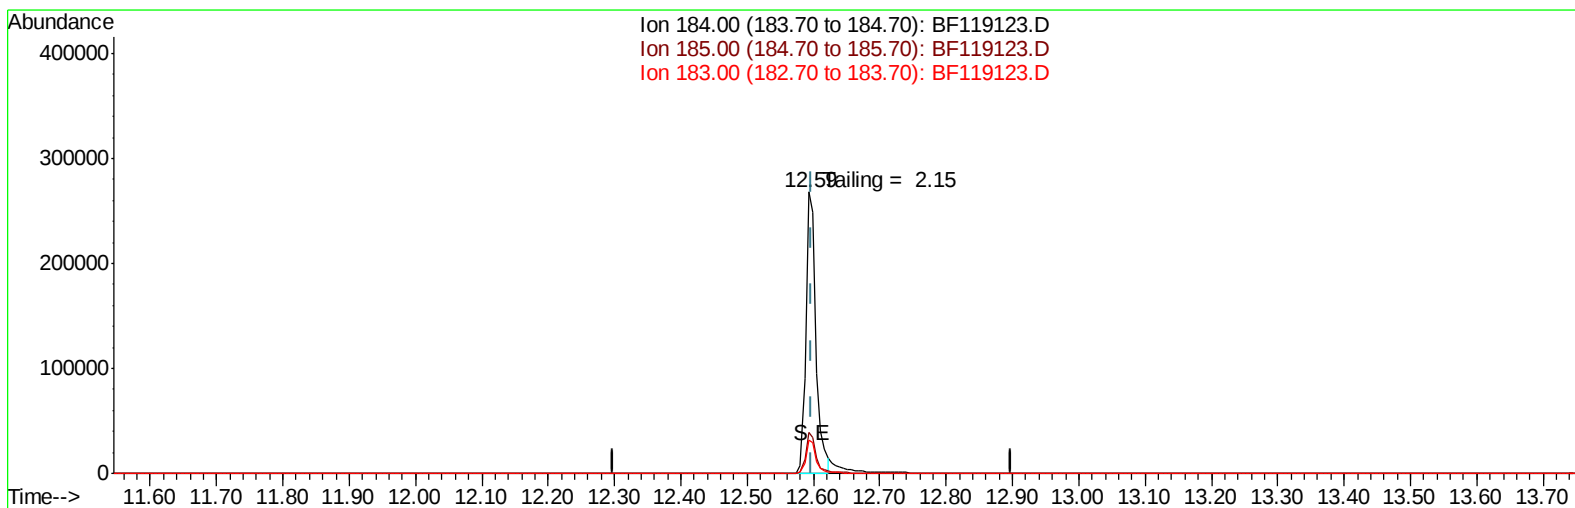

TIC: BF119123.D

(77) Benzidine

12.592min (-0.006) 0.00ng

response 297941

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.67
183.00	12.40	11.81
0.00	0.00	0.00