


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022720\
 Data File : BF119123.D
 Acq On : 27 Feb 2020 21:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 26 16:03:05 2020

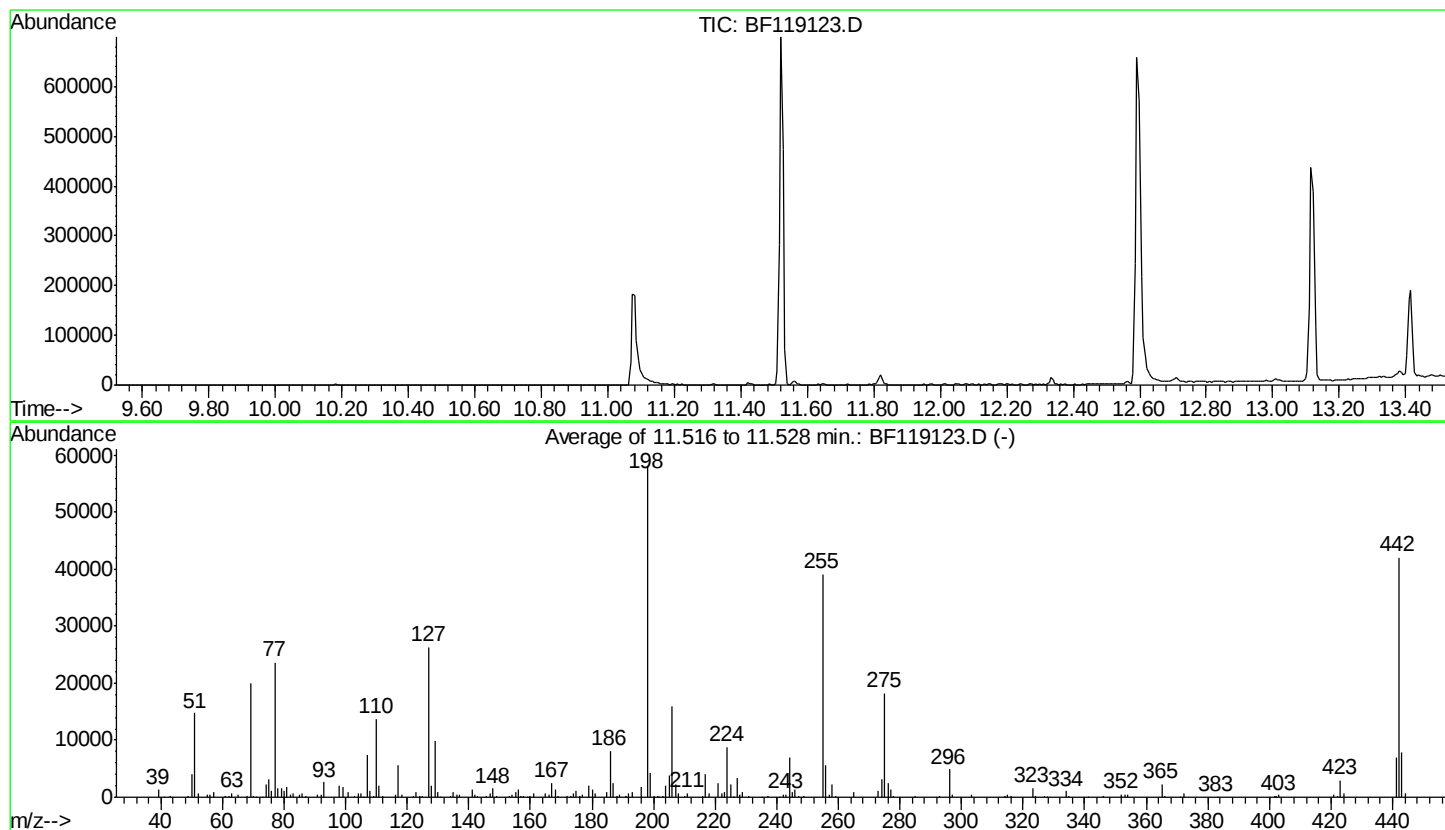

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	14733	PASS
68	69	0.00	2	0.6	124	PASS
69	198	0.00	100	34.3	19948	PASS
70	69	0.00	2	0.7	131	PASS
127	198	10	80	45.2	26264	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58146	PASS
199	198	5	9	7.2	4165	PASS
275	198	10	60	31.4	18244	PASS
365	198	1	100	4.0	2302	PASS
441	198	0.01	100	11.8	6858	PASS
442	198	50	100	72.3	42025	PASS
443	442	15	24	18.4	7753	PASS