
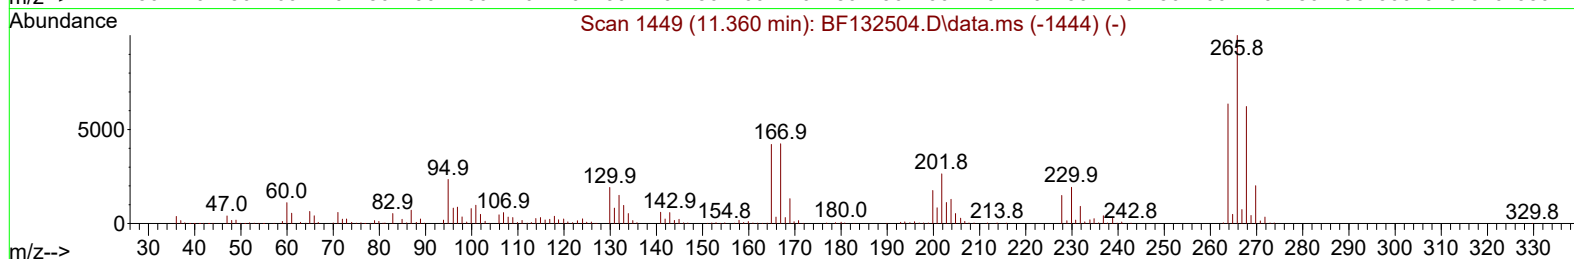
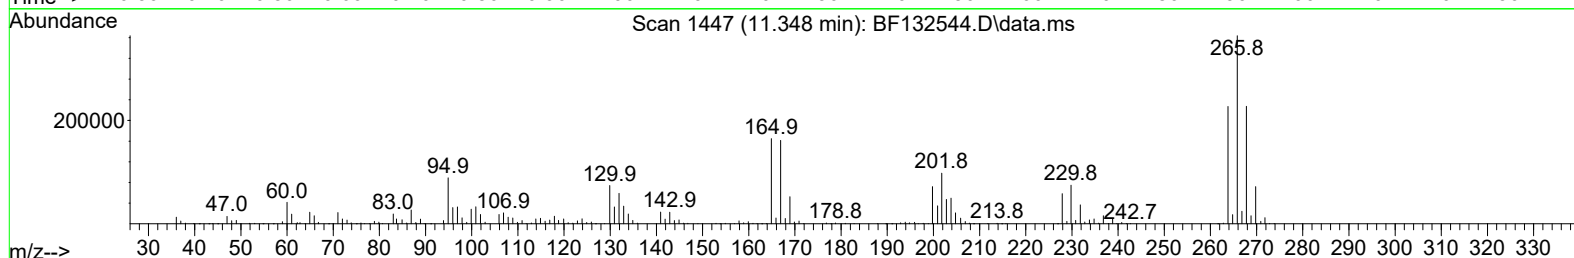


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022723\
Data File : BF132544.D
Acq On : 27 Feb 2023 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 04:11:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

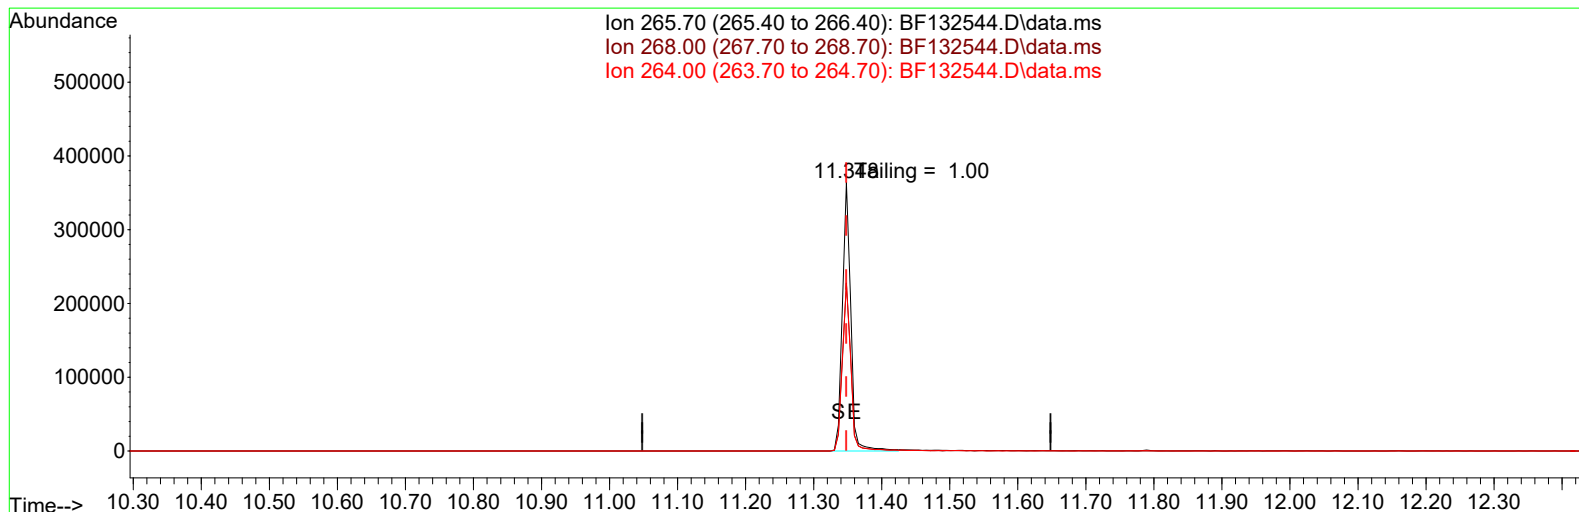

TIC: BF132544.D\data.ms

(70) Pentachlorophenol (C)




11.348min (+ 0.000) 237886.83 ng

response 313335

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.53
264.00	63.60	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022723\
Data File : BF132544.D
Acq On : 27 Feb 2023 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 04:11:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

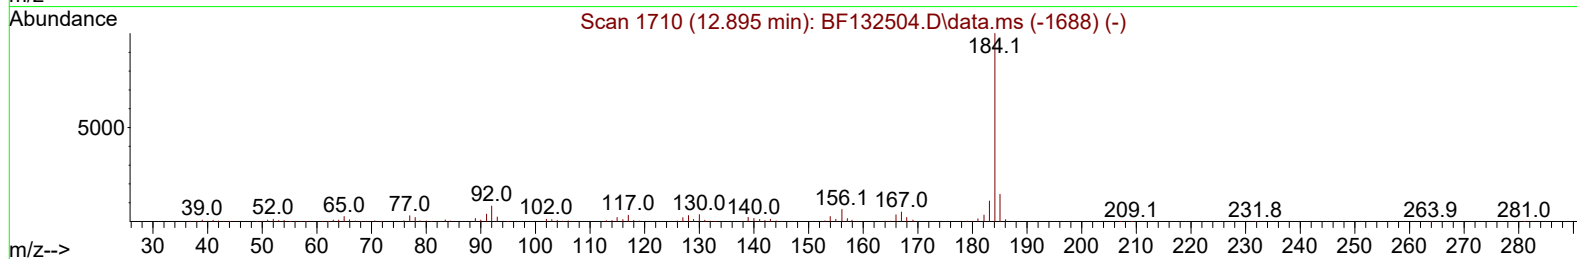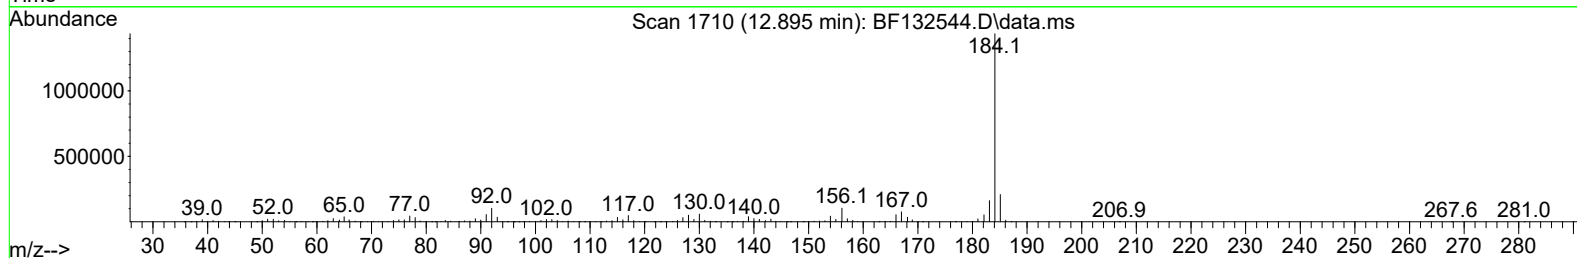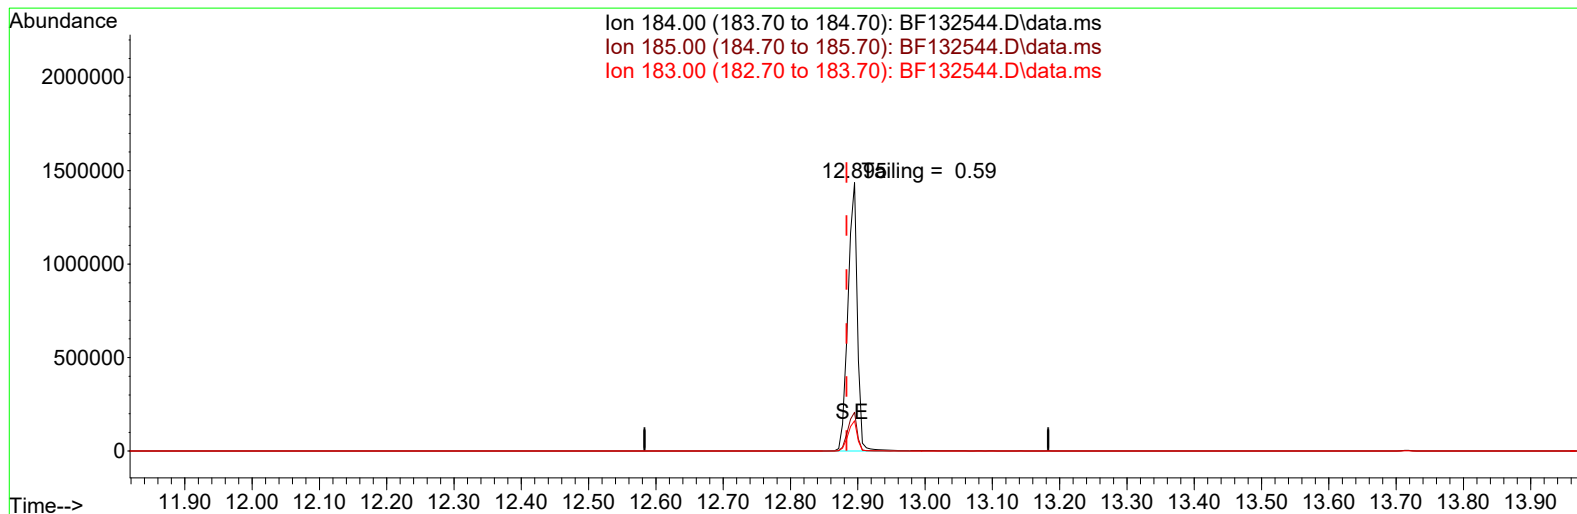

TIC: BF132544.D\data.ms

(77) Benzidine**12.895min (+ 0.012) 77645.03 ng****response 1391115**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.44
183.00	10.90	11.26
0.00	0.00	0.00