


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022723\
Data File : BF132544.D
Acq On : 27 Feb 2023 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 24 23:17:30 2023

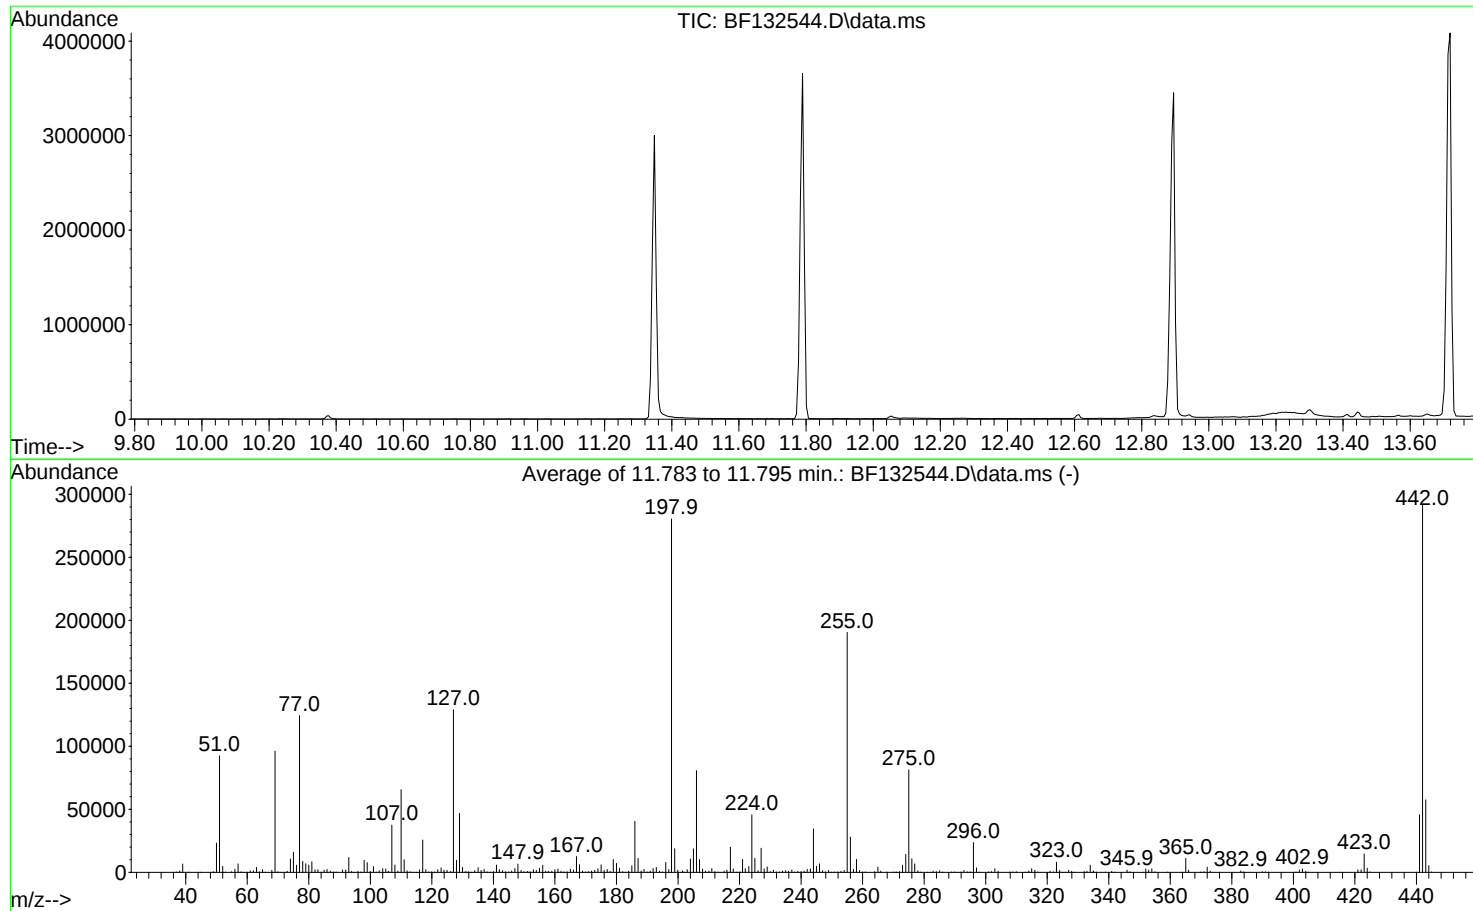




AutoFind: Scans 1521, 1522, 1523; Background Corrected with Scan 1516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	92403	PASS
68	69	0.00	2	1.7	1632	PASS
69	198	0.00	100	34.3	96192	PASS
70	69	0.00	2	0.5	464	PASS
127	198	10	80	46.0	128957	PASS
197	198	0.00	2	0.8	2208	PASS
198	198	100	100	100.0	280512	PASS
199	198	5	9	6.7	18682	PASS
275	198	10	60	29.0	81315	PASS
365	198	1	100	3.9	10992	PASS
441	198	0.01	100	16.3	45664	PASS
442	442	50	100	100.0	291947	PASS
443	442	15	24	19.7	57533	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022723\
Data File : BF132544.D
Acq On : 27 Feb 2023 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 28 04:11:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

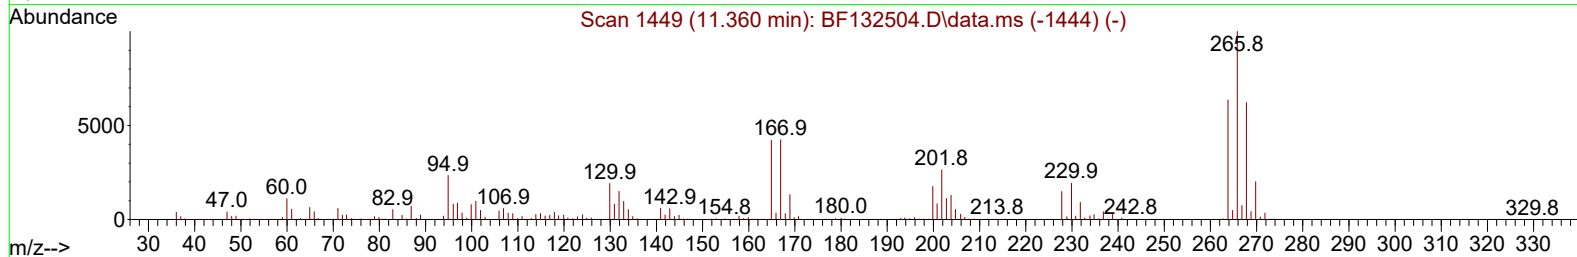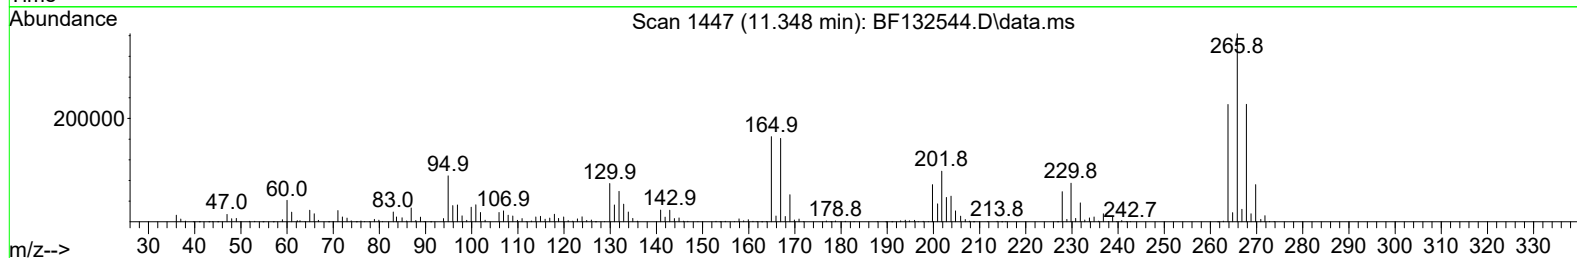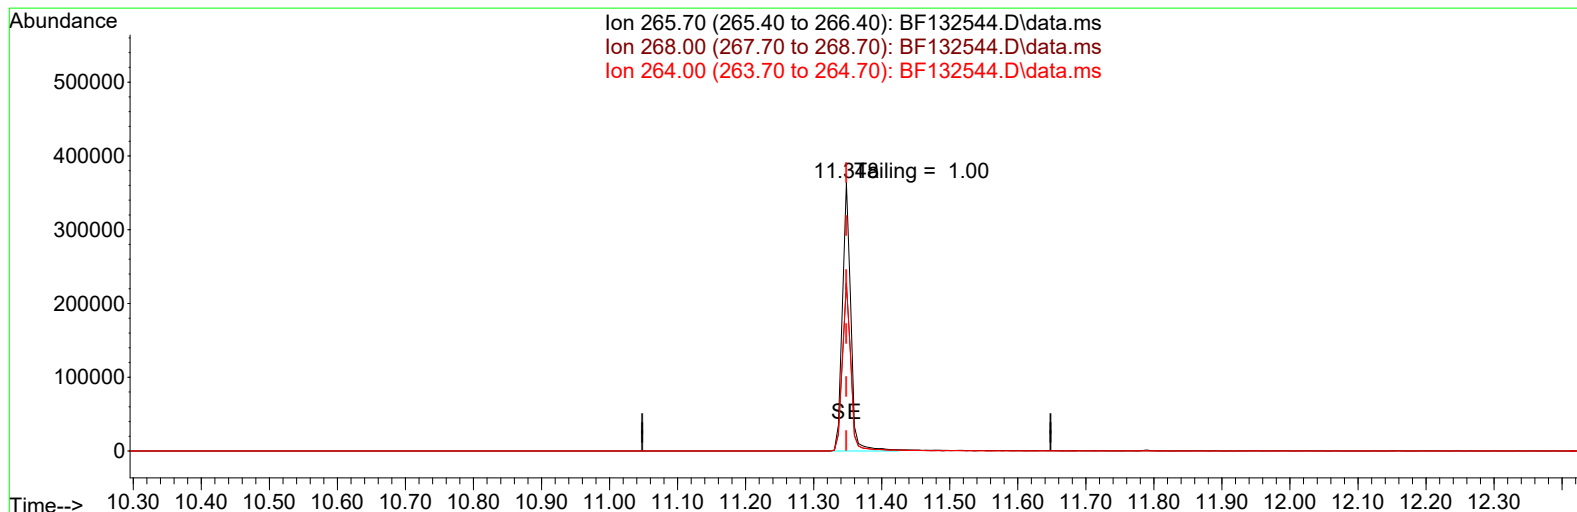

TIC: BF132544.D\data.ms

(70) Pentachlorophenol (C)

11.348min (+ 0.000) 237886.83 ng




response 313335

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.53
264.00	63.60	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022723\
Data File : BF132544.D
Acq On : 27 Feb 2023 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 28 04:11:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

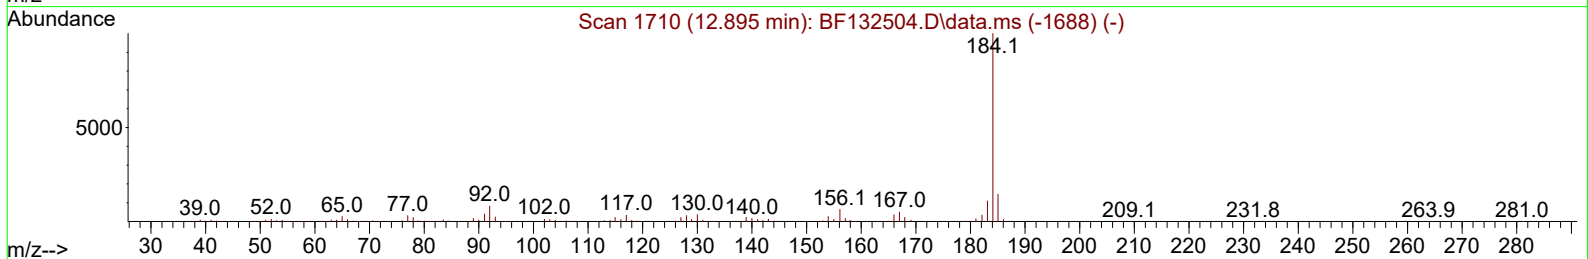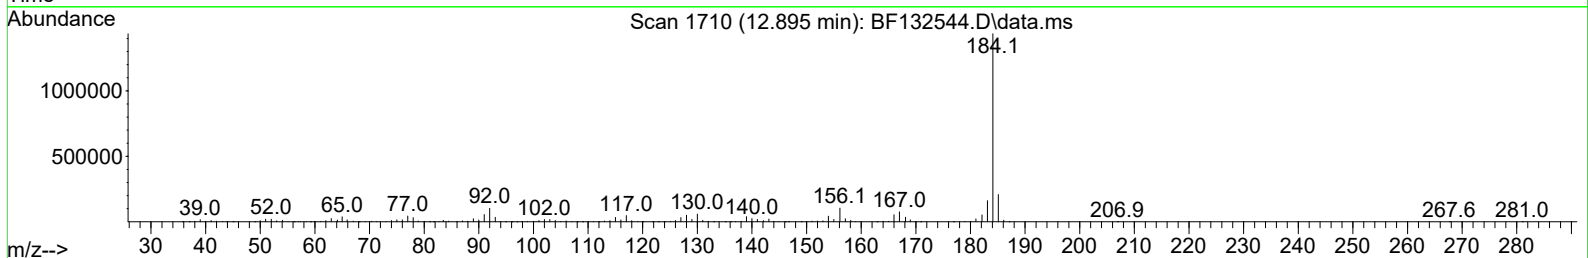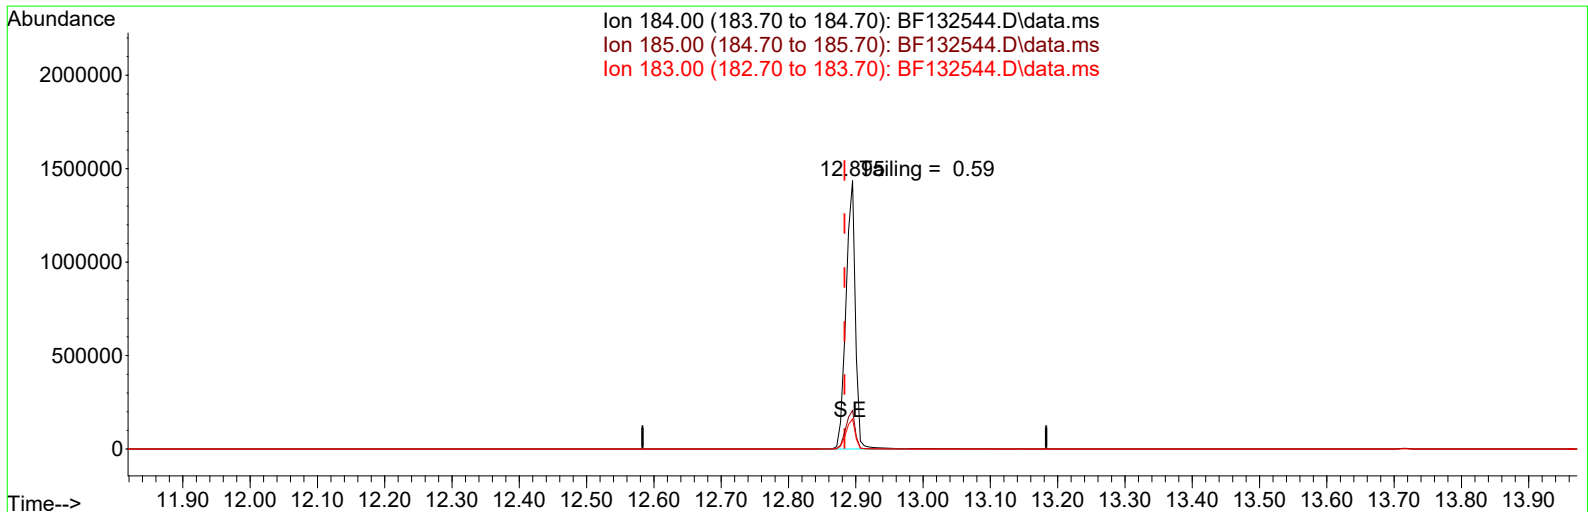

TIC: BF132544.D\data.ms

(77) Benzidine

12.895min (+ 0.012) 77645.03 ng

response 1391115

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.44
183.00	10.90	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/27/2023	BNA_F	<u>BF132544.D</u>
Compound Name	Response	Retention Time
DDT	791090	13.719
DDD	16157	13.442
DDE	1439	13.072
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17596	808686	2.18

Instrument :
BNA_F
ClientSampleId :
DFTPP