
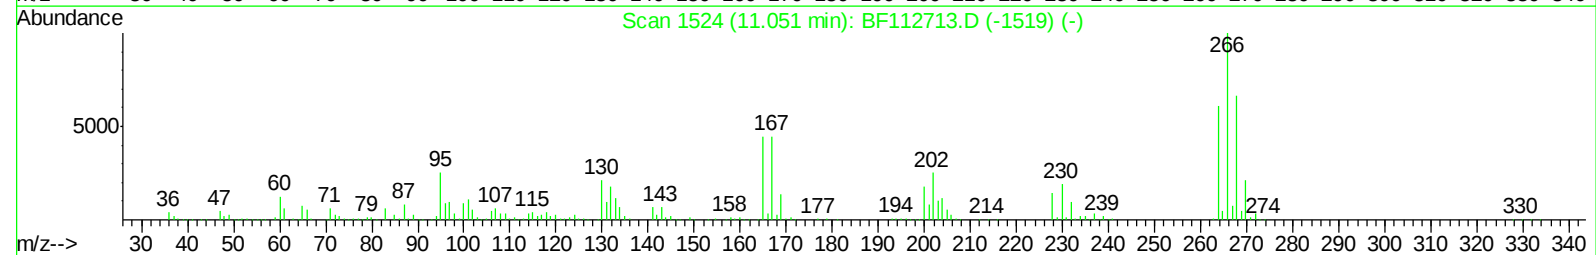
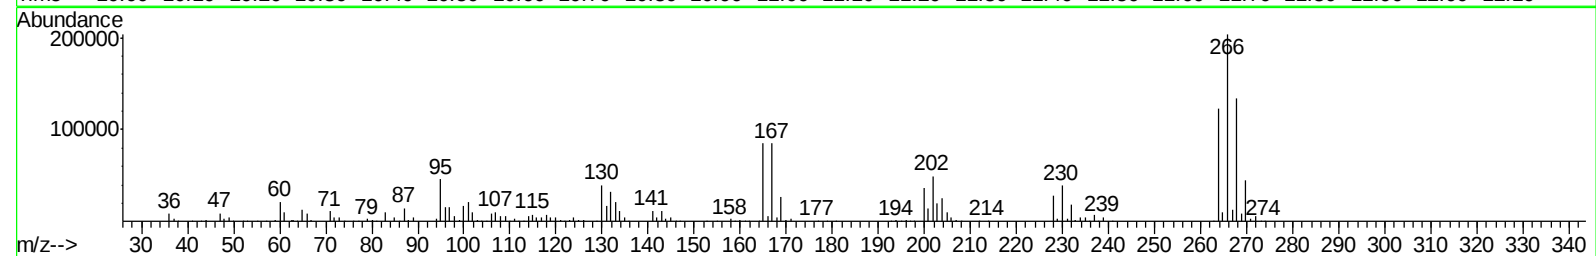


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022819\
Data File : BF112751.D
Acq On : 28 Feb 2019 10:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 09:02:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 27 16:08:50 2019
Response via : Initial Calibration

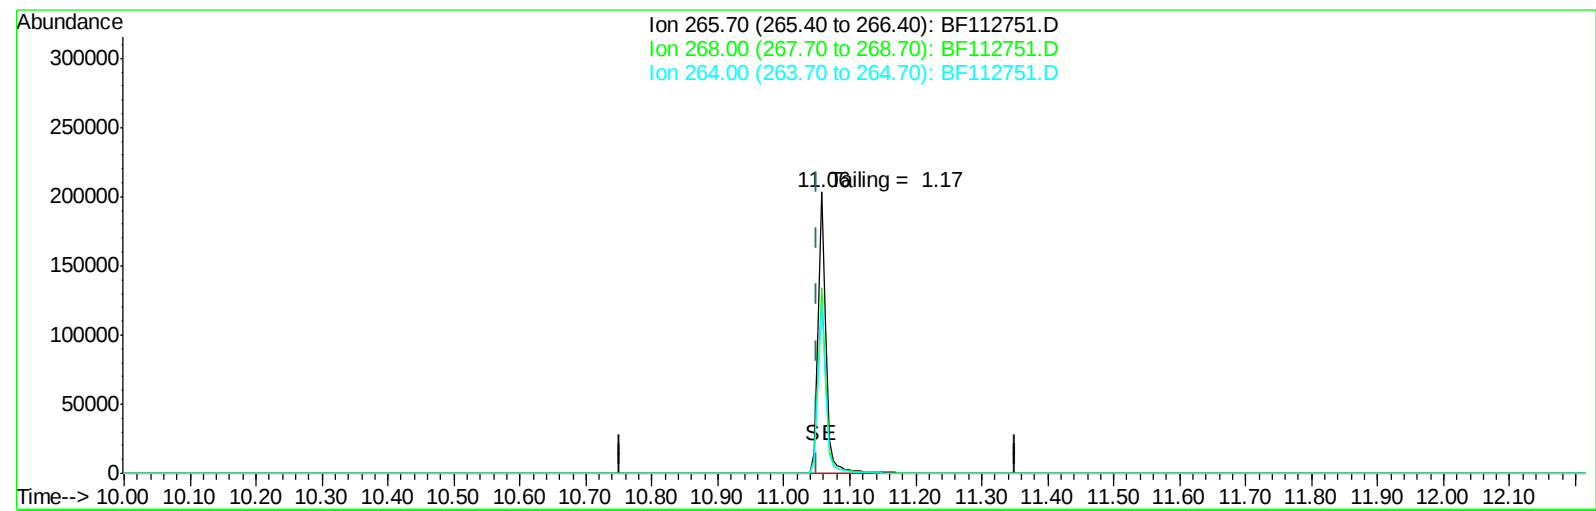

TIC: BF112751.D

(70) Pentachlorophenol (C)




11.057min (+0.006) 0.00ng

response 173393

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.07
264.00	61.10	60.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022819\
Data File : BF112751.D
Acq On : 28 Feb 2019 10:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 09:02:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 27 16:08:50 2019
Response via : Initial Calibration

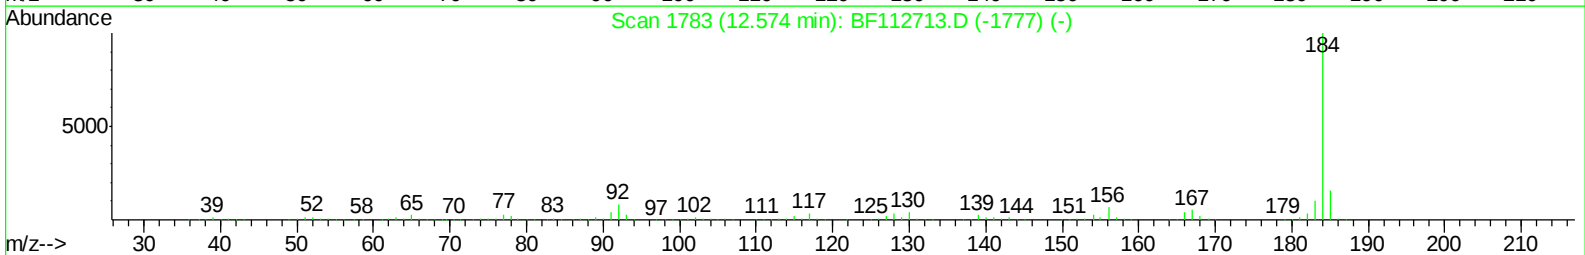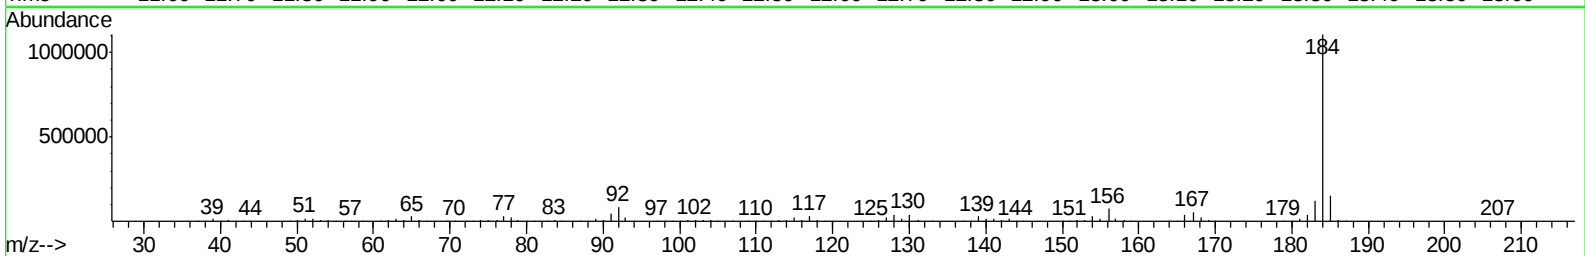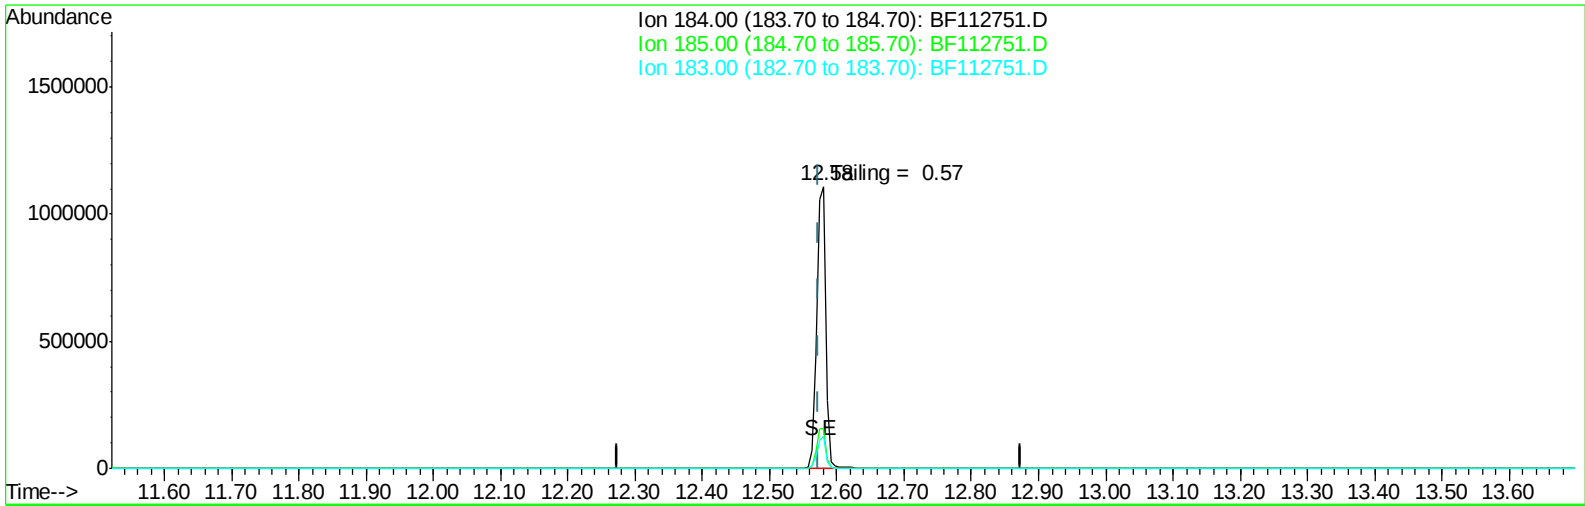

TIC: BF112751.D

(77) Benzidine

12.580min (+0.006) 92869.10ng

response 1064824

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.02
183.00	10.70	11.18
0.00	0.00	0.00