
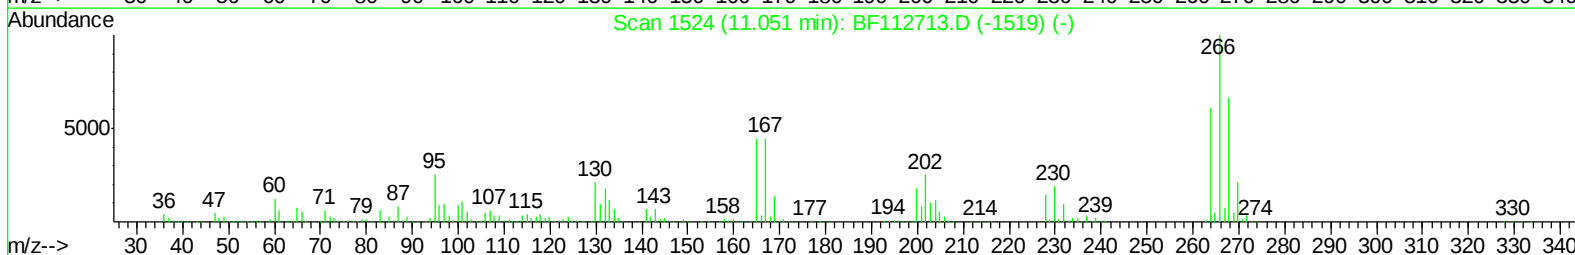
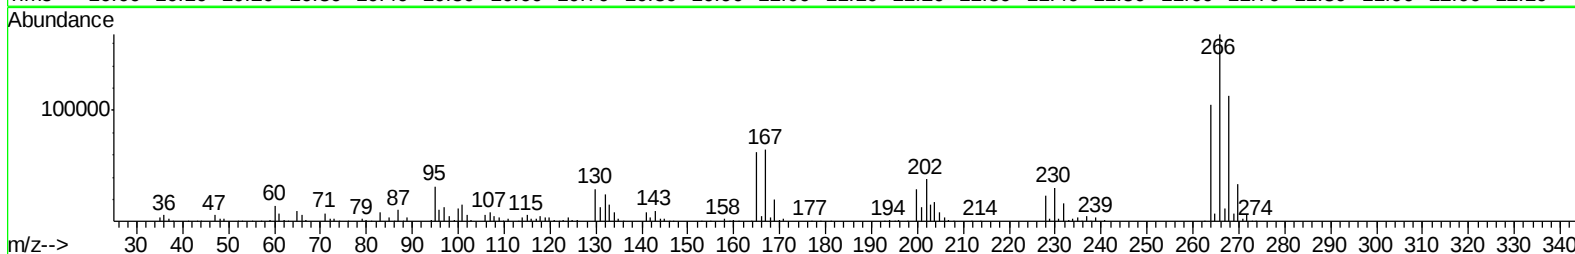


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022819\
Data File : BF112765.D
Acq On : 28 Feb 2019 17:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 09:20:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 27 16:08:50 2019
Response via : Initial Calibration

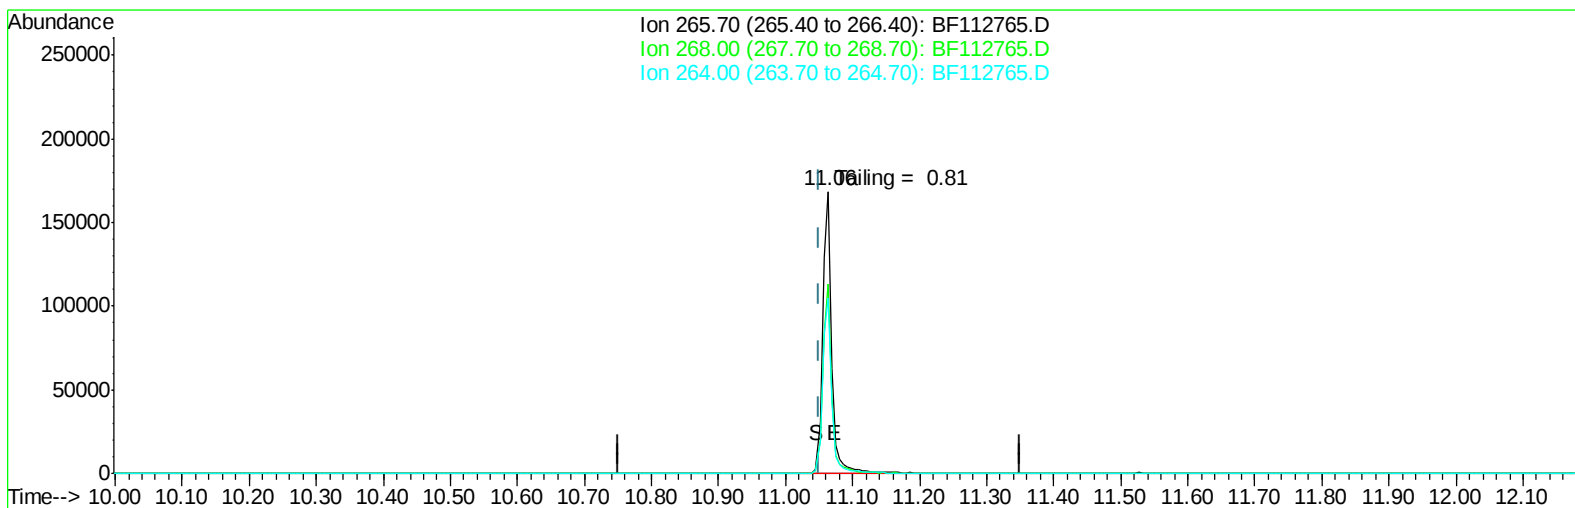

TIC: BF112765.D

(70) Pentachlorophenol (C)




11.063min (+0.012) 202183.57ng

response 156836

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.47
264.00	61.10	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022819\
 Data File : BF112765.D
 Acq On : 28 Feb 2019 17:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 09:20:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 27 16:08:50 2019
 Response via : Initial Calibration

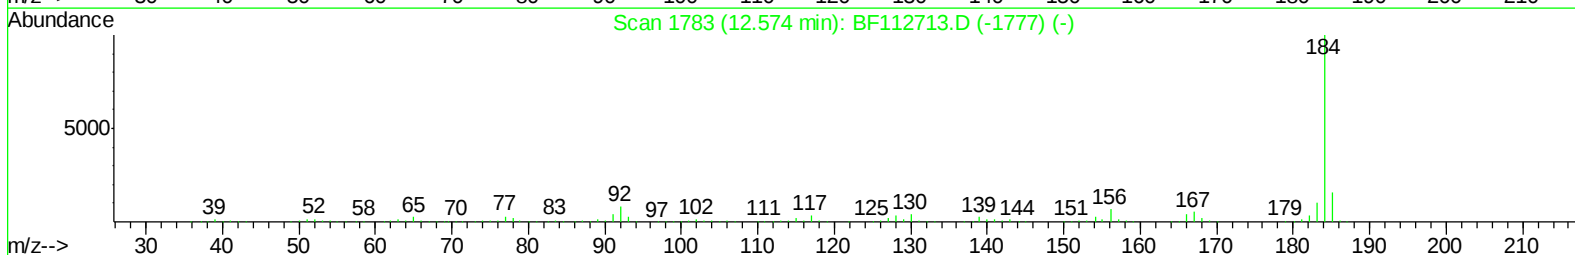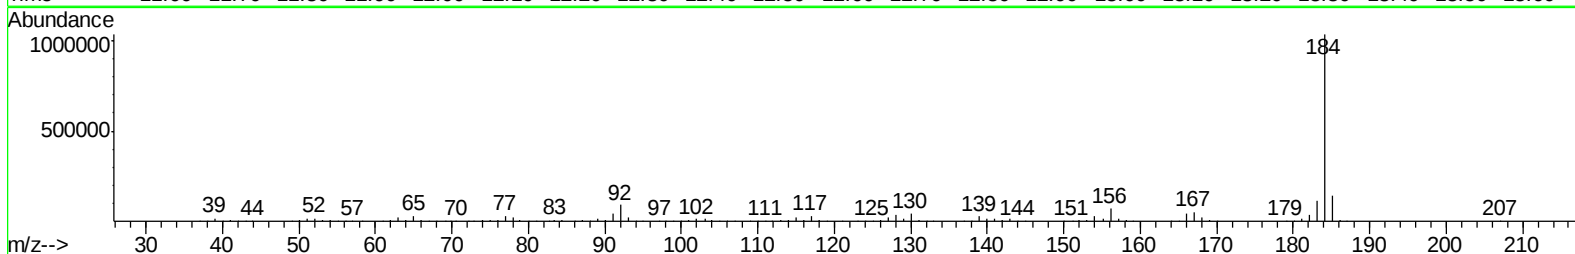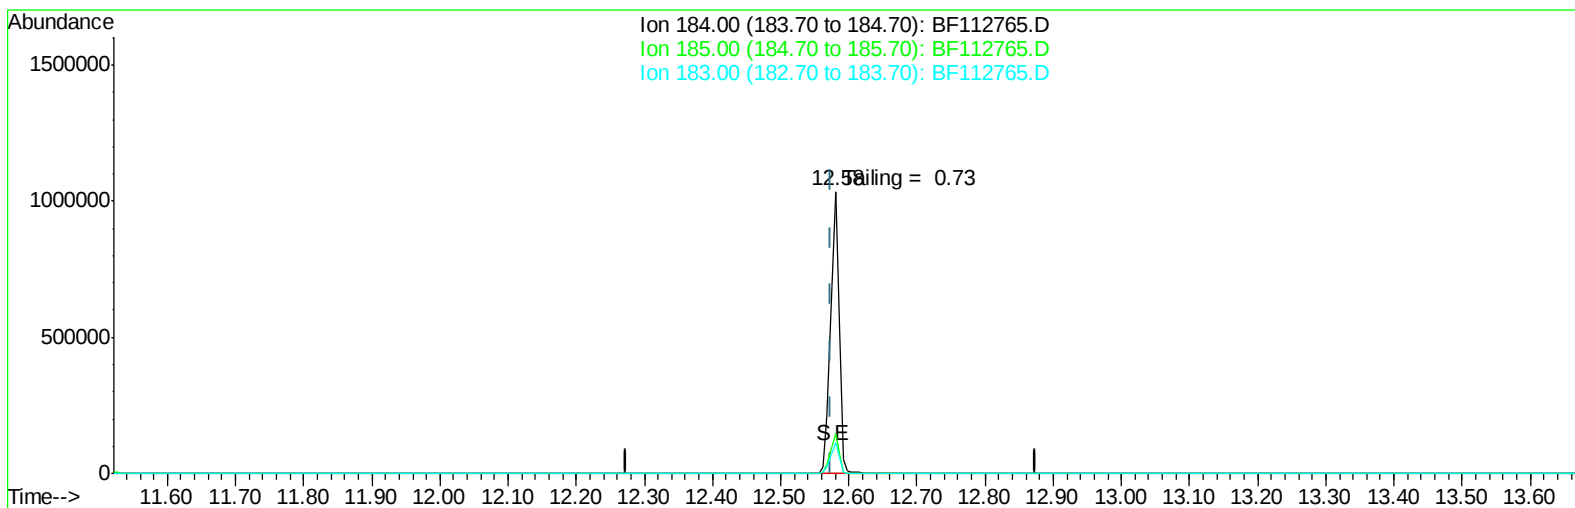

TIC: BF112765.D

(77) Benzidine

12.580min (+0.006) 38482.13ng

response 908416

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.94
183.00	10.70	11.06
0.00	0.00	0.00