


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022819\
 Data File : BF112765.D
 Acq On : 28 Feb 2019 17:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 15:40:43 2019

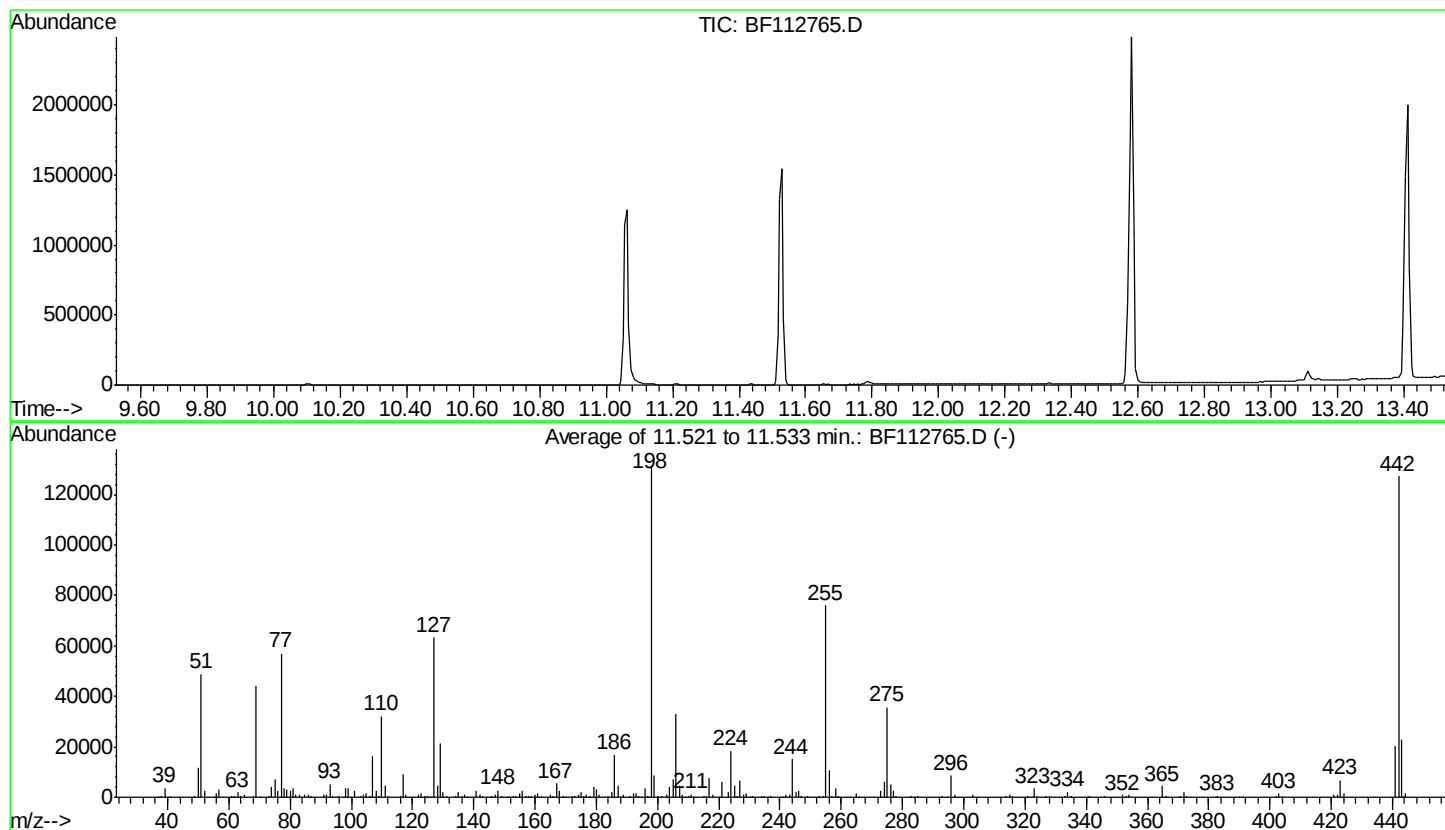

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	48754	PASS
68	69	0.00	2	1.7	758	PASS
69	198	0.00	100	33.5	43987	PASS
70	69	0.00	2	0.5	234	PASS
127	198	10	80	48.2	63317	PASS
197	198	0.00	2	0.2	283	PASS
198	198	100	100	100.0	131448	PASS
199	198	5	9	6.7	8854	PASS
275	198	10	60	27.2	35778	PASS
365	198	1	100	3.3	4339	PASS
441	198	0.01	100	15.6	20540	PASS
442	198	50	100	96.9	127357	PASS
443	442	15	24	18.1	22997	PASS