
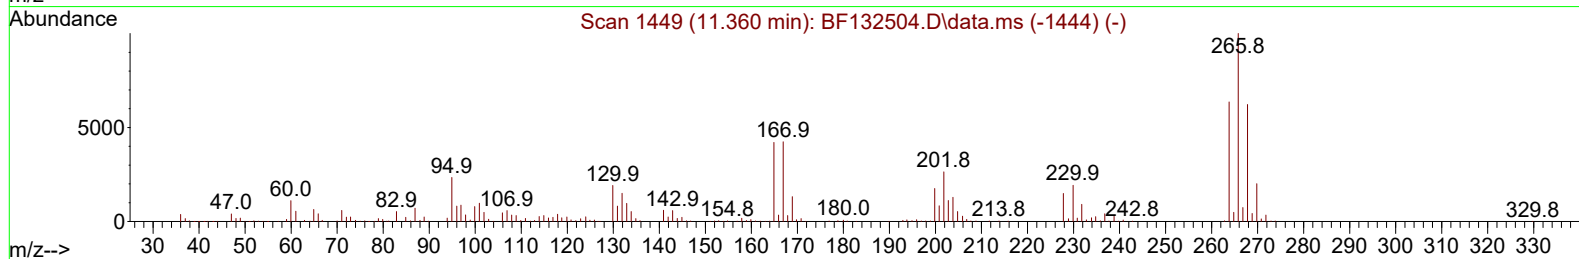
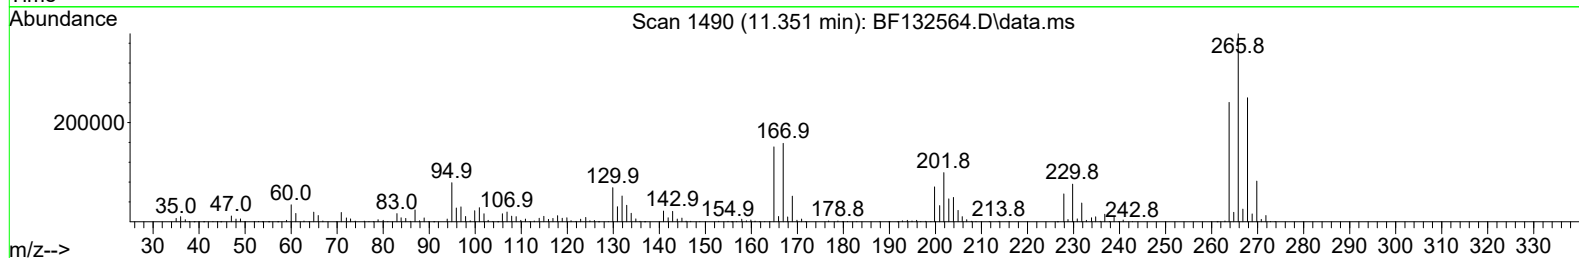


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132564.D
Acq On : 28 Feb 2023 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 04:27:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

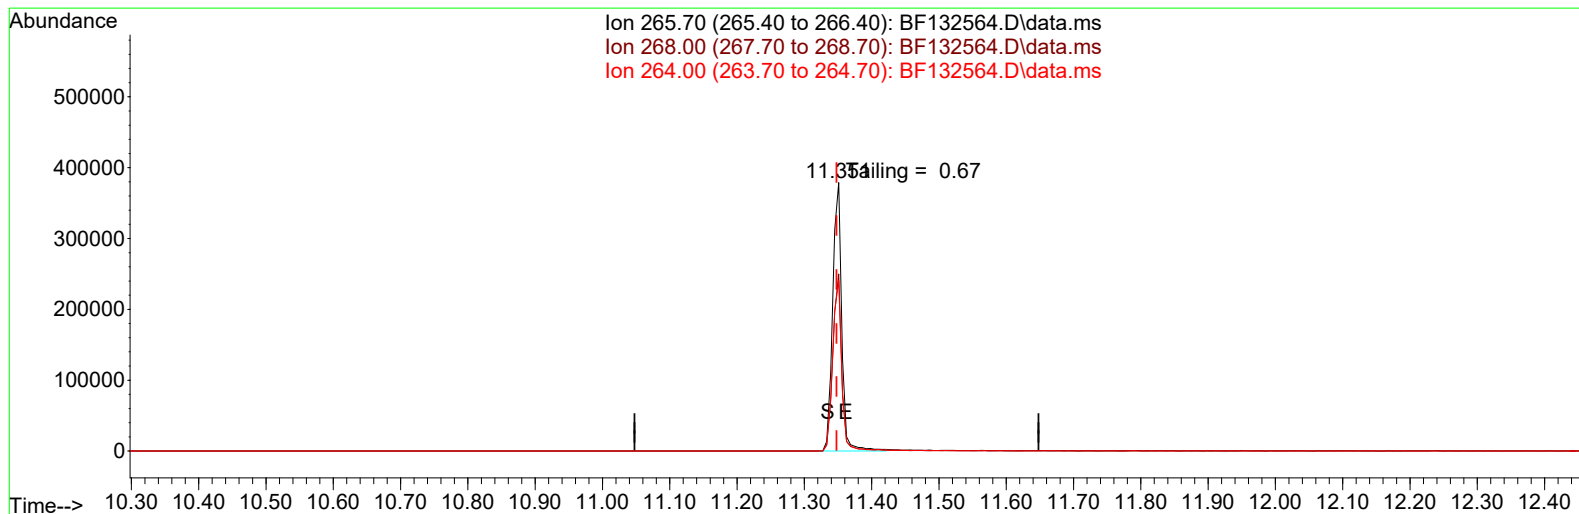

TIC: BF132564.D\data.ms

(70) Pentachlorophenol (C)




11.351min (+ 0.003) 857385.03 ng

response 358223

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.96
264.00	63.60	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132564.D
Acq On : 28 Feb 2023 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 04:27:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

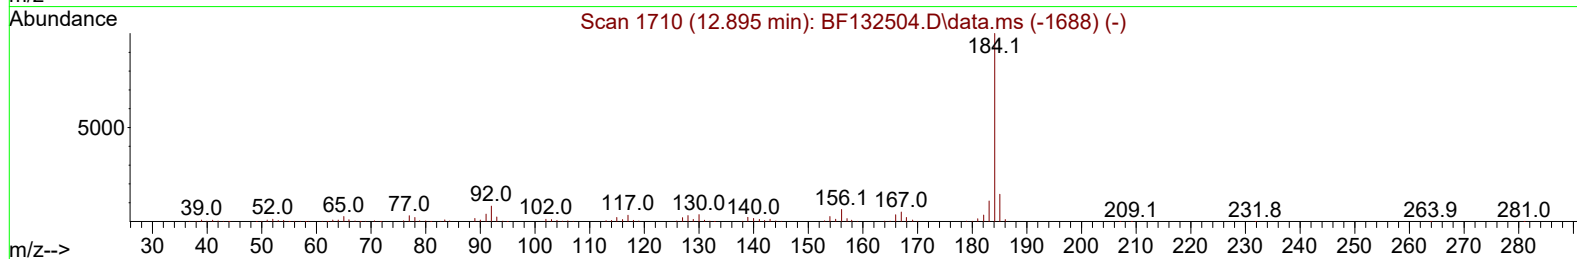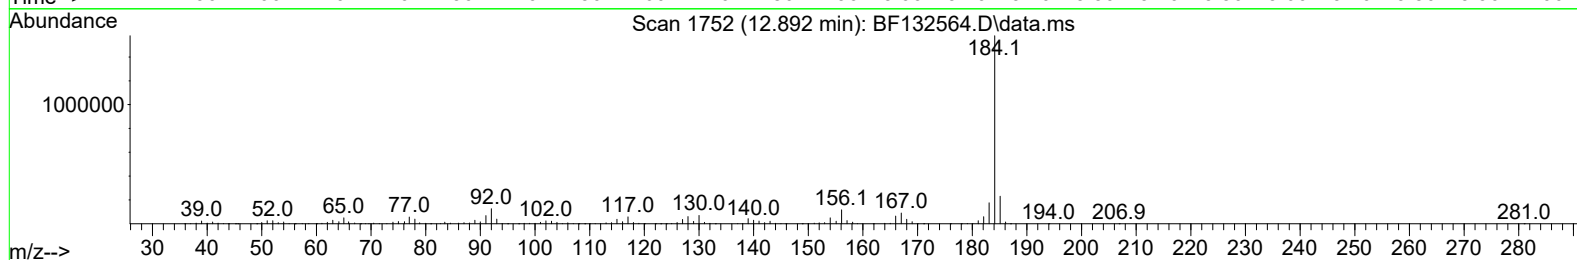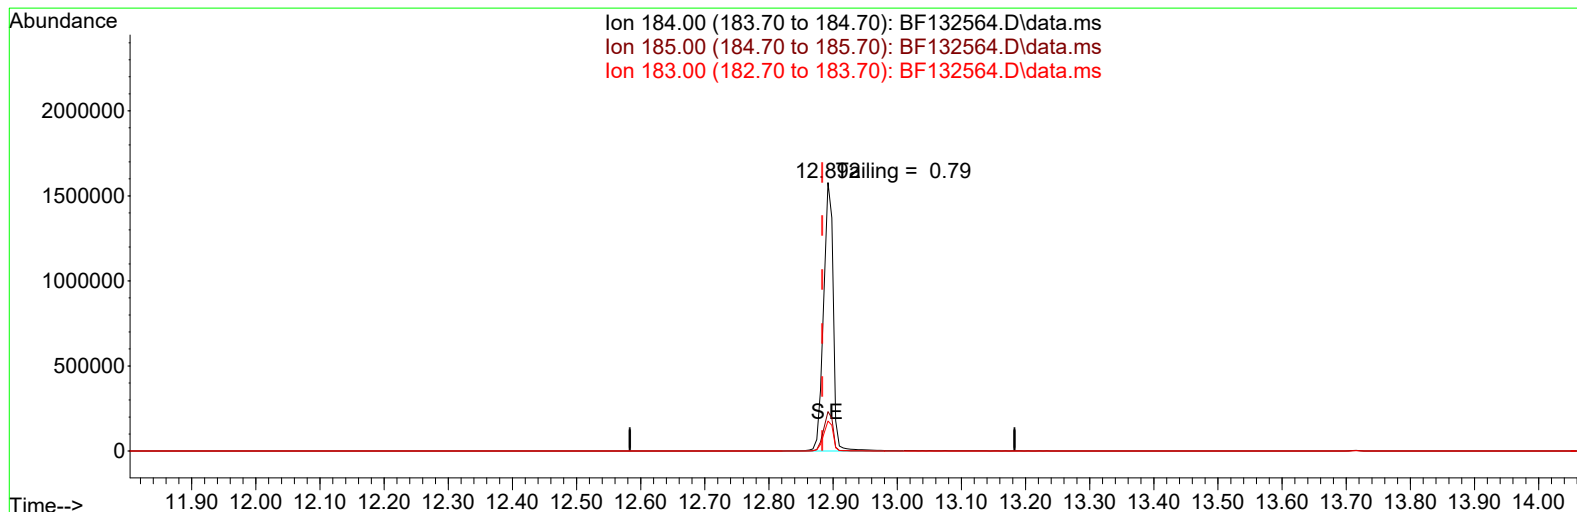

TIC: BF132564.D\data.ms

(77) Benzidine**12.892min (+ 0.009) 1053622.00 ng****response 1667131**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.66
183.00	10.90	11.17
0.00	0.00	0.00