

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
 Data File : BF132581.D
 Acq On : 28 Feb 2023 20:01
 Operator : CG\JU
 Sample : 01727-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JB1-WATER

Quant Time: Mar 01 02:30:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 23:17:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.998	152	237616	20.000	ng	0.00
21) Naphthalene-d8	8.287	136	881042	20.000	ng	0.00
39) Acenaphthene-d10	10.051	164	472458	20.000	ng	0.00
64) Phenanthrene-d10	11.545	188	915262	20.000	ng	0.00
76) Chrysene-d12	14.198	240	584659	20.000	ng	# 0.00
86) Perylene-d12	15.751	264	434558	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.628	112	951123	64.964	ng	0.00
7) Phenol-d6	6.622	99	753072	39.412	ng	-0.01
23) Nitrobenzene-d5	7.569	82	1597363	86.018	ng	0.00
42) 2,4,6-Tribromophenol	10.845	330	672756	131.852	ng	0.00
45) 2-Fluorobiphenyl	9.363	172	2436180	78.514	ng	0.00
79) Terphenyl-d14	13.139	244	2939229	84.998	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132581.D
Acq On : 28 Feb 2023 20:01
Operator : CG\JU
Sample : 01727-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JB1-WATER

Quant Time: Mar 01 02:30:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration




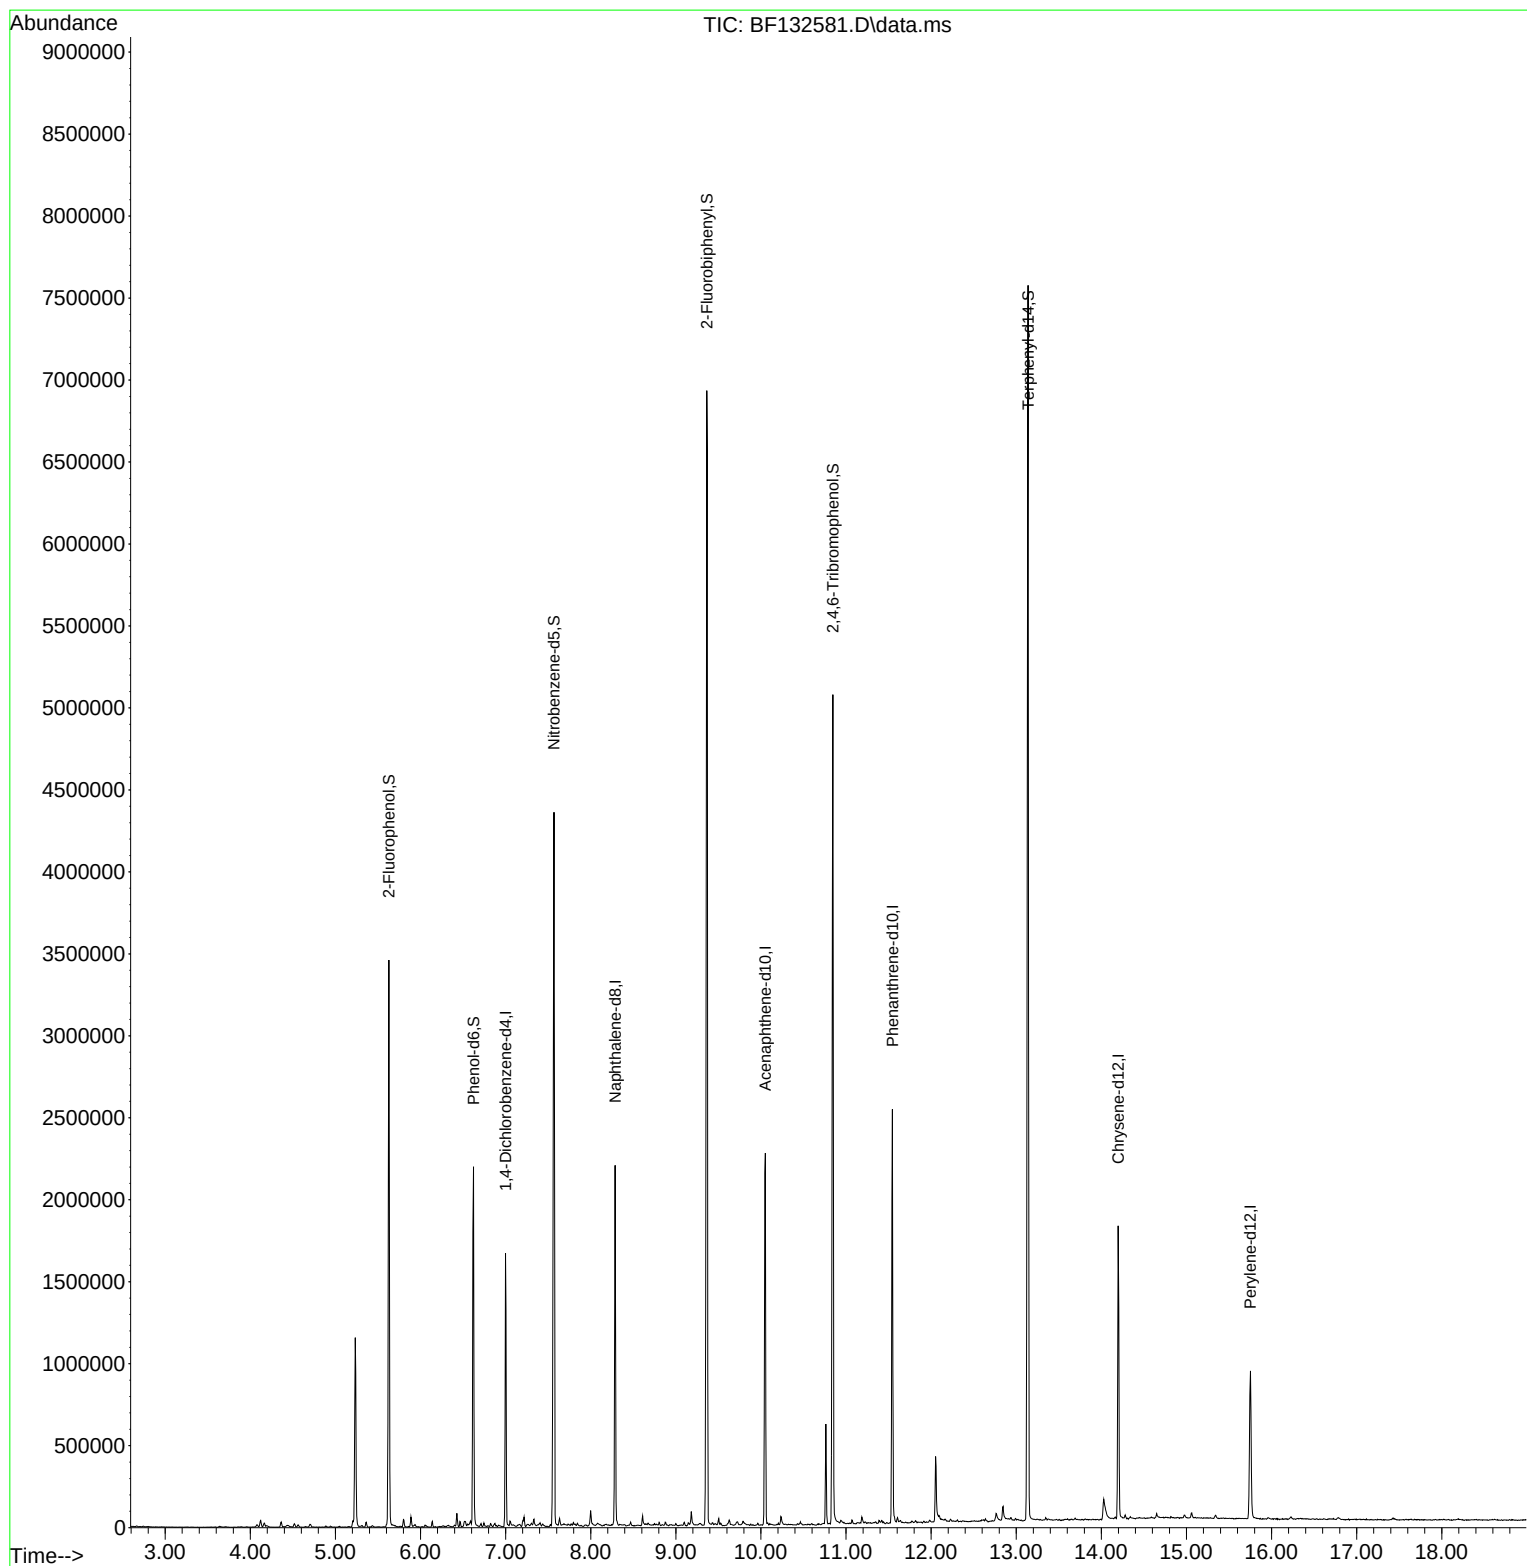


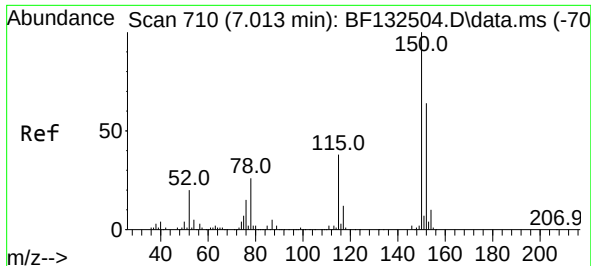

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.998 min Scan# 710
 Delta R.T. -0.009 min
 Lab File: BF132581.D
 Acq: 28 Feb 2023 20:01




Instrument :
 BNA_F
 ClientSampleId :
 JB1-WATER


Tgt Ion:152 Resp: 237616
 Ion Ratio Lower Upper
 152 100
 150 160.3 125.4 188.2
 115 64.5 47.8 71.6

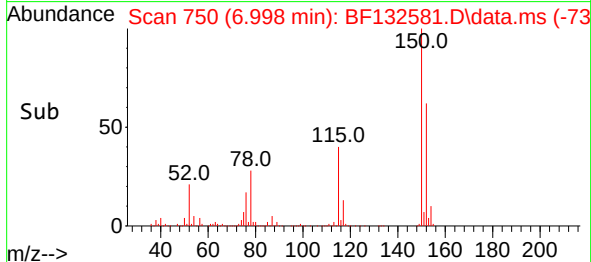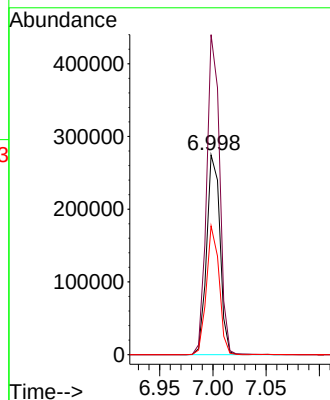

#5
 2-Fluorophenol
 Concen: 64.964 ng
 RT: 5.628 min Scan# 517
 Delta R.T. -0.003 min
 Lab File: BF132581.D
 Acq: 28 Feb 2023 20:01

Tgt Ion:112 Resp: 951123
 Ion Ratio Lower Upper
 112 100
 64 59.2 51.6 77.4
 63 30.3 27.4 41.2


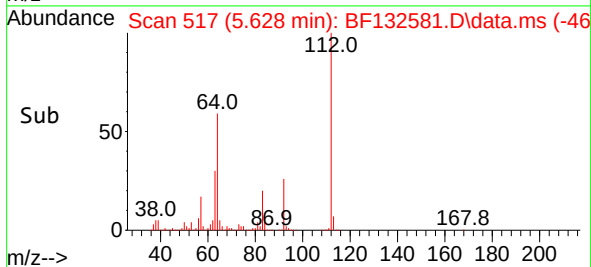
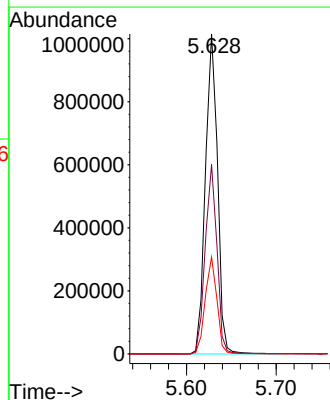
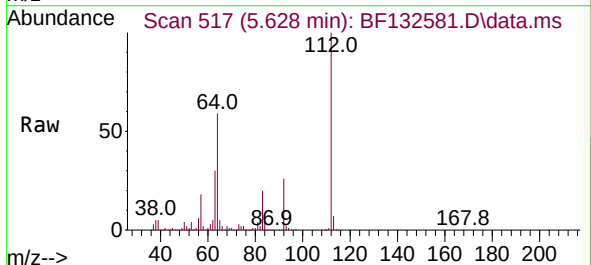




#7
Phenol-d6
Concen: 39.412 ng
RT: 6.622 min Scan# 686
Delta R.T. -0.015 min
Lab File: BF132581.D
Acq: 28 Feb 2023 20:01




Instrument :
BNA_F
ClientSampleId :
JB1-WATER


Tgt Ion: 99 Resp: 753072
Ion Ratio Lower Upper
99 100
42 13.9 13.9 20.9
71 30.7 28.5 42.7

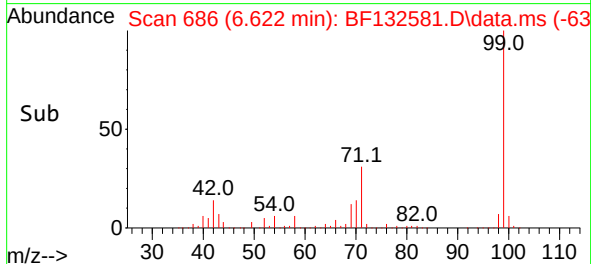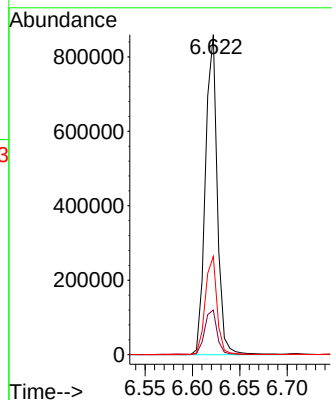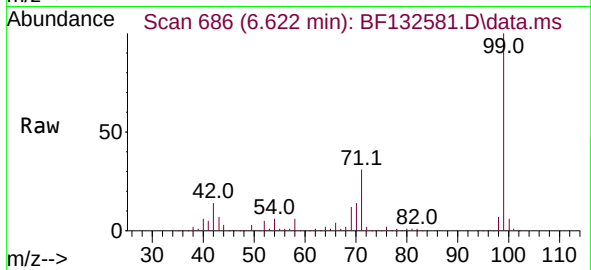

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.287 min Scan# 969
Delta R.T. -0.003 min
Lab File: BF132581.D
Acq: 28 Feb 2023 20:01

Tgt Ion: 136 Resp: 881042
Ion Ratio Lower Upper
136 100
137 11.2 8.9 13.3
54 7.8 6.2 9.4
68 6.9 5.2 7.8


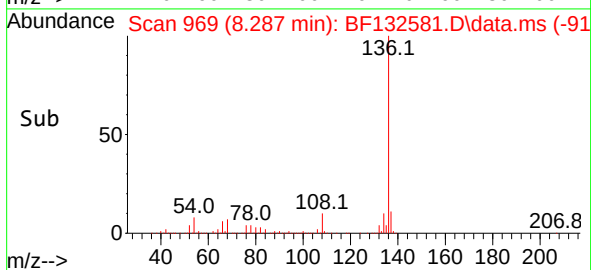
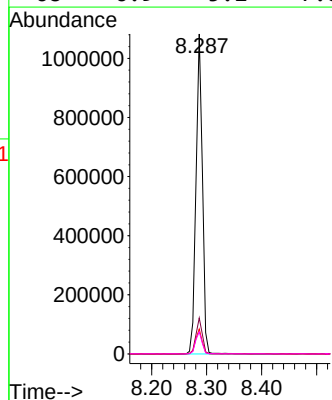
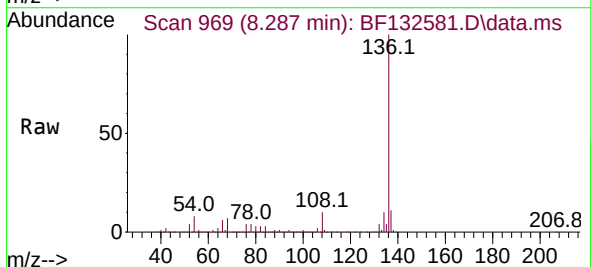




#23
Nitrobenzene-d5
Concen: 86.018 ng
RT: 7.569 min Scan# 84
Delta R.T. -0.003 min
Lab File: BF132581.D
Acq: 28 Feb 2023 20:01




Instrument :
BNA_F
ClientSampleId :
JB1-WATER


Tgt Ion: 82 Resp: 1597363
Ion Ratio Lower Upper
82 100
128 41.0 32.2 48.2
54 45.1 38.4 57.6

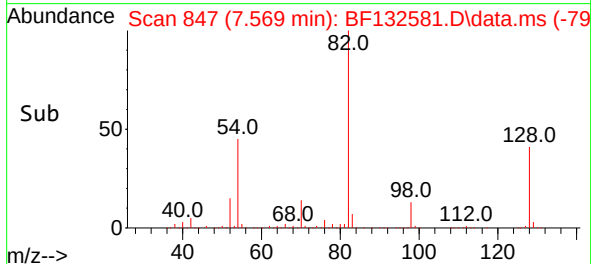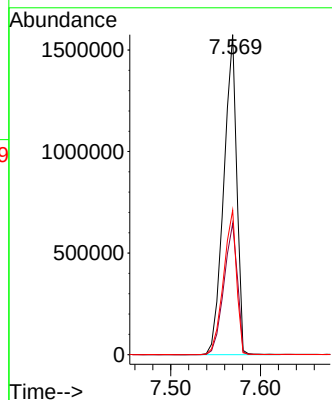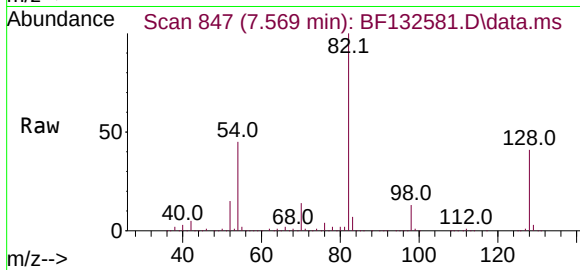

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.051 min Scan# 1269
Delta R.T. -0.003 min
Lab File: BF132581.D
Acq: 28 Feb 2023 20:01

Tgt Ion:164 Resp: 472458
Ion Ratio Lower Upper
164 100
162 102.7 79.8 119.8
160 45.9 35.8 53.6

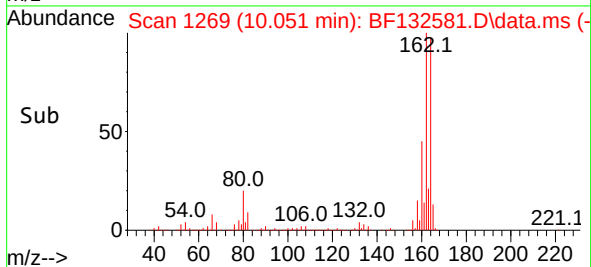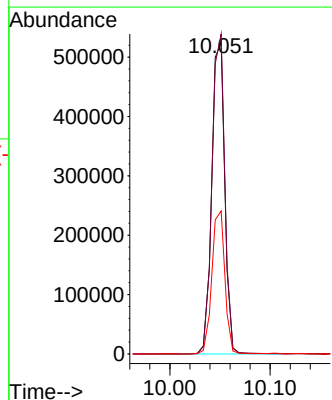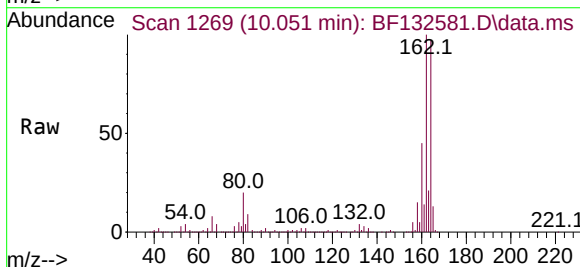

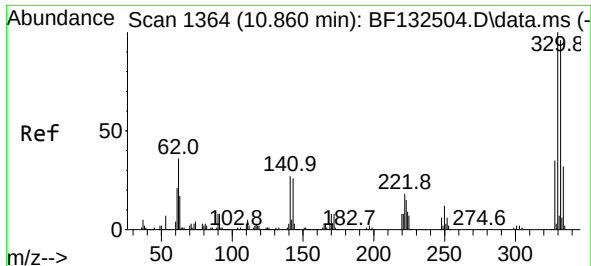

#42

2,4,6-Tribromophenol

Concen: 131.852 ng

RT: 10.845 min Scan# 1404

Delta R.T. -0.003 min

Lab File: BF132581.D


Acq: 28 Feb 2023 20:01

Instrument :

BNA_F

ClientSampleId :

JB1-WATER






Tgt Ion:330 Resp: 672756

Ion Ratio Lower Upper

330 100

332 95.6 76.2 114.4

141 33.3 28.4 42.6

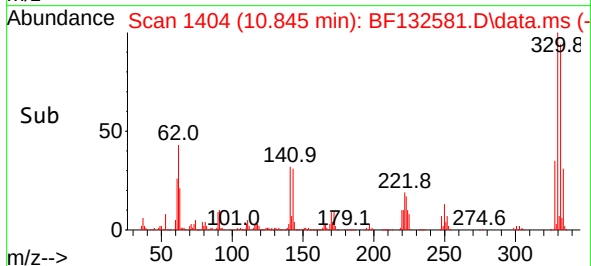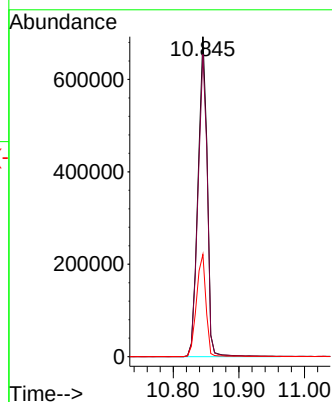

#45

2-Fluorobiphenyl

Concen: 78.514 ng

RT: 9.363 min Scan# 1152

Delta R.T. -0.009 min

Lab File: BF132581.D

Acq: 28 Feb 2023 20:01




Tgt Ion:172 Resp: 2436180


Ion Ratio Lower Upper

172 100

171 35.6 28.8 43.2

170 24.4 19.7 29.5

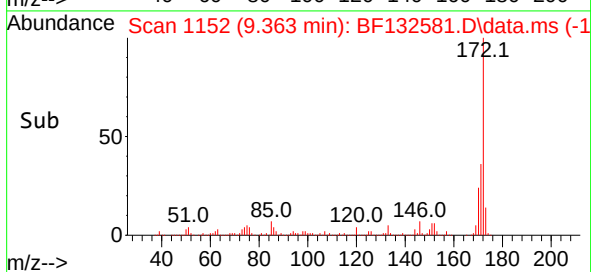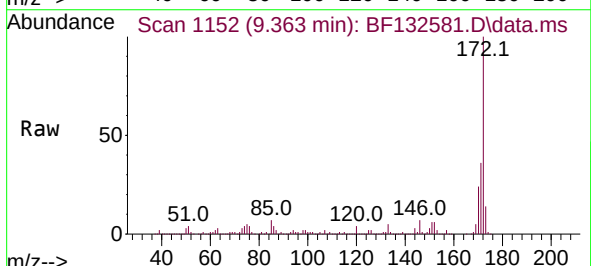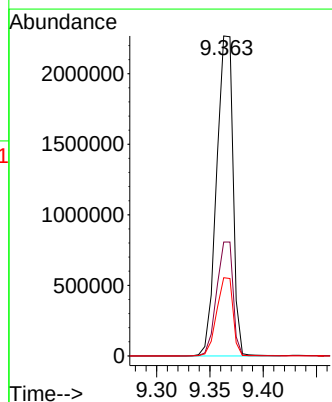

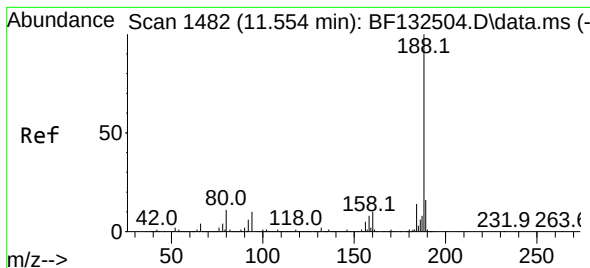

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.545 min Scan# 11

Delta R.T. -0.003 min

Lab File: BF132581.D

Acq: 28 Feb 2023 20:01

Instrument :

BNA_F

ClientSampleId :

JB1-WATER





Tgt Ion:188 Resp: 915262

Ion Ratio Lower Upper

188 100

94 9.7 8.3 12.5

80 10.0 8.7 13.1

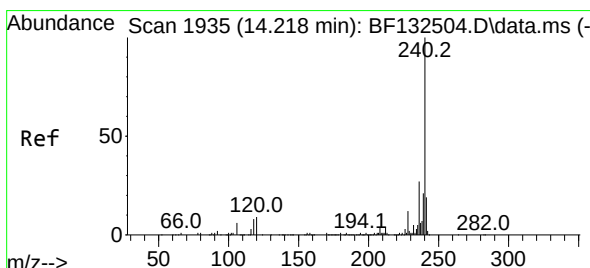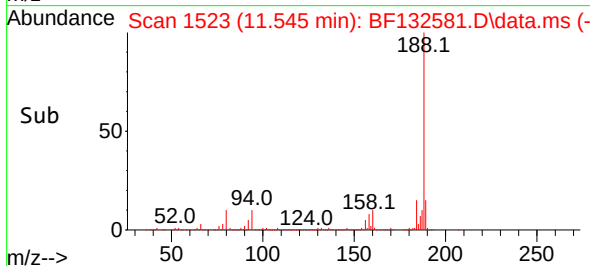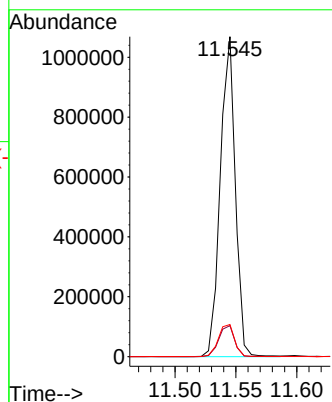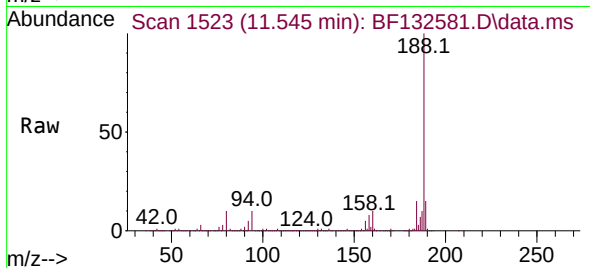

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.198 min Scan# 1974

Delta R.T. -0.009 min

Lab File: BF132581.D

Acq: 28 Feb 2023 20:01




Tgt Ion:240 Resp: 584659


Ion Ratio Lower Upper

240 100

120 11.5 7.2 10.8#

236 27.1 21.8 32.6

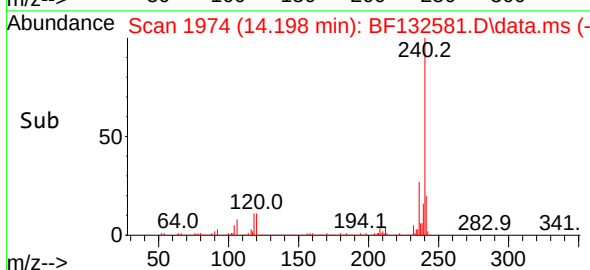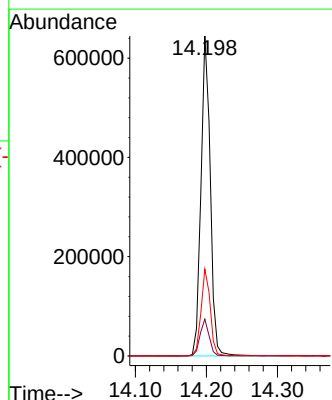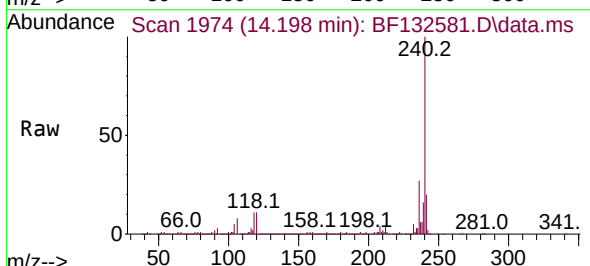



#79

Terphenyl-d14

Concen: 84.998 ng

RT: 13.139 min Scan# 11

Delta R.T. -0.003 min

Lab File: BF132581.D

Acq: 28 Feb 2023 20:01

Instrument :

BNA_F

ClientSampleId :

JB1-WATER





Tgt Ion:244 Resp: 2939229

Ion Ratio Lower Upper

244 100

212 8.3 6.5 9.7

122 9.1 7.5 11.3

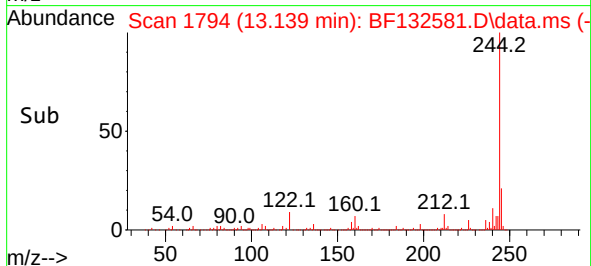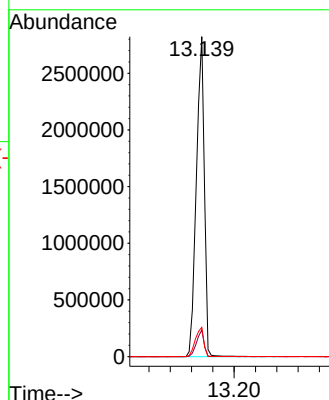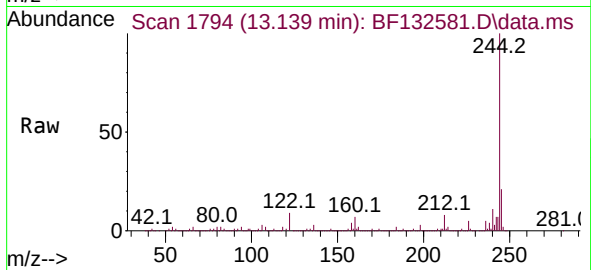

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.751 min Scan# 2238

Delta R.T. -0.003 min

Lab File: BF132581.D

Acq: 28 Feb 2023 20:01

Tgt Ion:264 Resp: 434558

Ion Ratio Lower Upper

264 100

260 24.8 18.8 28.2

265 21.9 17.1 25.7

