

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
 Data File : BF132571.D
 Acq On : 28 Feb 2023 14:40
 Operator : CG\JU
 Sample : 01703-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KU-CON1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.646	341	350	355	rBV	1355775	1520232	30.86%	4.219%
2	5.251	446	453	456	rVB	2305097	3008417	61.06%	8.349%
3	5.634	514	518	521	rBV	3344134	3084818	62.61%	8.561%
4	6.016	580	583	589	rBV	89904	81631	1.66%	0.227%
5	6.628	682	687	690	rBV	3403849	3313760	67.26%	9.196%
6	7.004	747	751	754	rBV	1222679	1070230	21.72%	2.970%
7	7.569	841	847	850	rBV	2460775	2427442	49.27%	6.737%
8	8.286	965	969	972	rBV	1719052	1378217	27.97%	3.825%
9	9.363	1146	1152	1155	rBV	5054226	4407348	89.45%	12.231%
10	10.051	1265	1269	1272	rBV	1856262	1598831	32.45%	4.437%
11	10.763	1386	1390	1393	rBV	1139334	905748	18.38%	2.514%
12	10.845	1399	1404	1407	rBV	2543354	2538034	51.51%	7.044%
13	10.939	1417	1420	1425	rBV3	39190	61263	1.24%	0.170%
14	11.075	1440	1443	1446	rBV	116268	110138	2.24%	0.306%
15	11.422	1498	1502	1508	rVB	62421	71648	1.45%	0.199%
16	11.545	1519	1523	1526	rBV	2021462	1712859	34.76%	4.753%
17	12.051	1604	1609	1617	rBV	387949	463875	9.41%	1.287%
18	12.204	1632	1635	1637	rBV2	72275	67350	1.37%	0.187%
19	12.845	1739	1744	1751	rBV	134936	184080	3.74%	0.511%
20	13.139	1789	1794	1797	rBV	5332239	4927013	100.00%	13.673%
21	14.027	1941	1945	1959	rBV2	219788	439197	8.91%	1.219%
22	14.204	1970	1975	1978	rBV	1432338	1401082	28.44%	3.888%
23	14.439	2012	2015	2023	rVB4	39853	60439	1.23%	0.168%
24	14.980	2103	2107	2111	rVB2	39404	52835	1.07%	0.147%
25	15.345	2165	2169	2176	rVB	60387	83821	1.70%	0.233%
26	15.751	2233	2238	2246	rVB	771988	1063359	21.58%	2.951%




Sum of corrected areas: 36033667

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132571.D
Acq On : 28 Feb 2023 14:40
Operator : CG\JU
Sample : 01703-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KU-CON1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

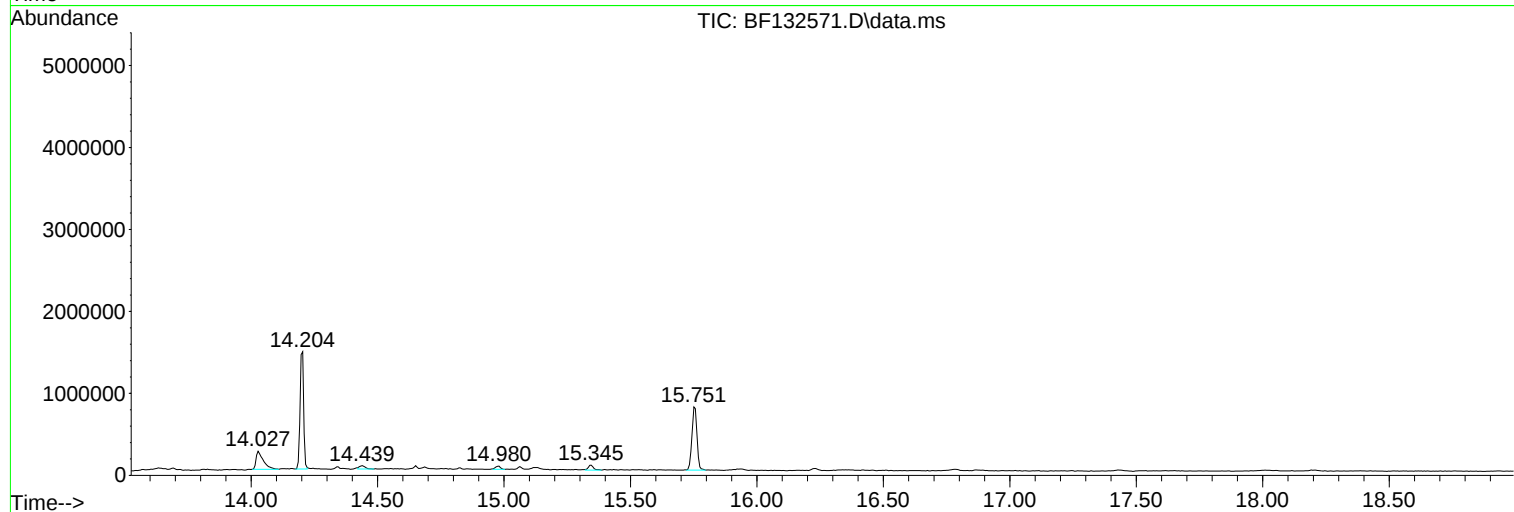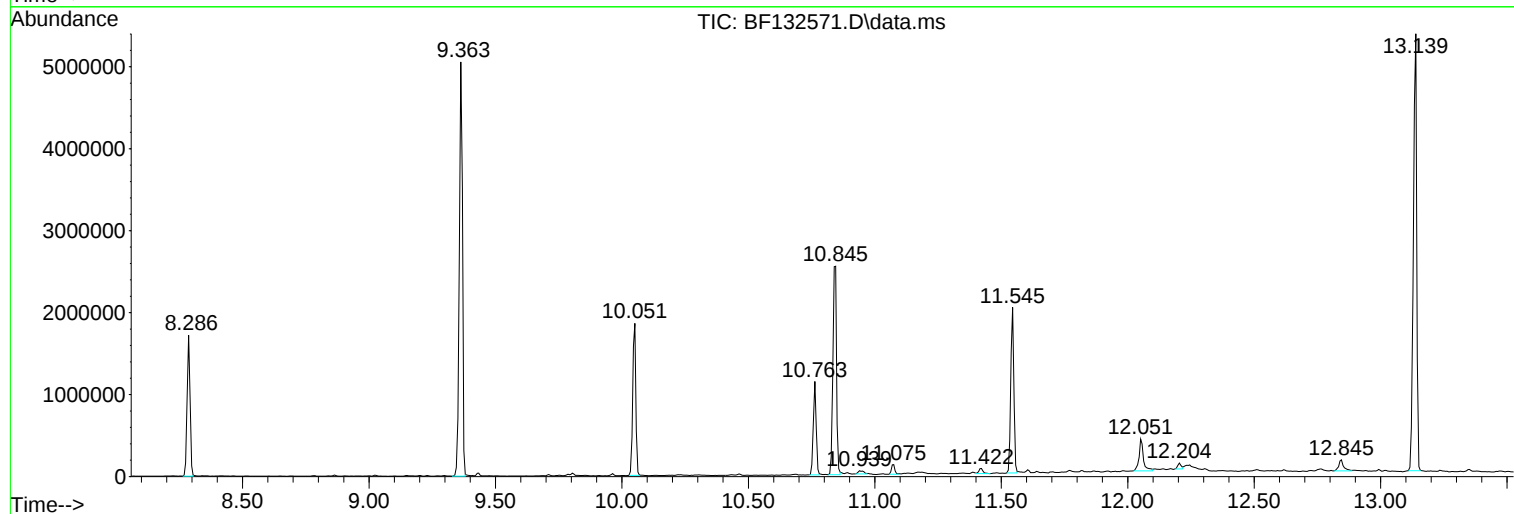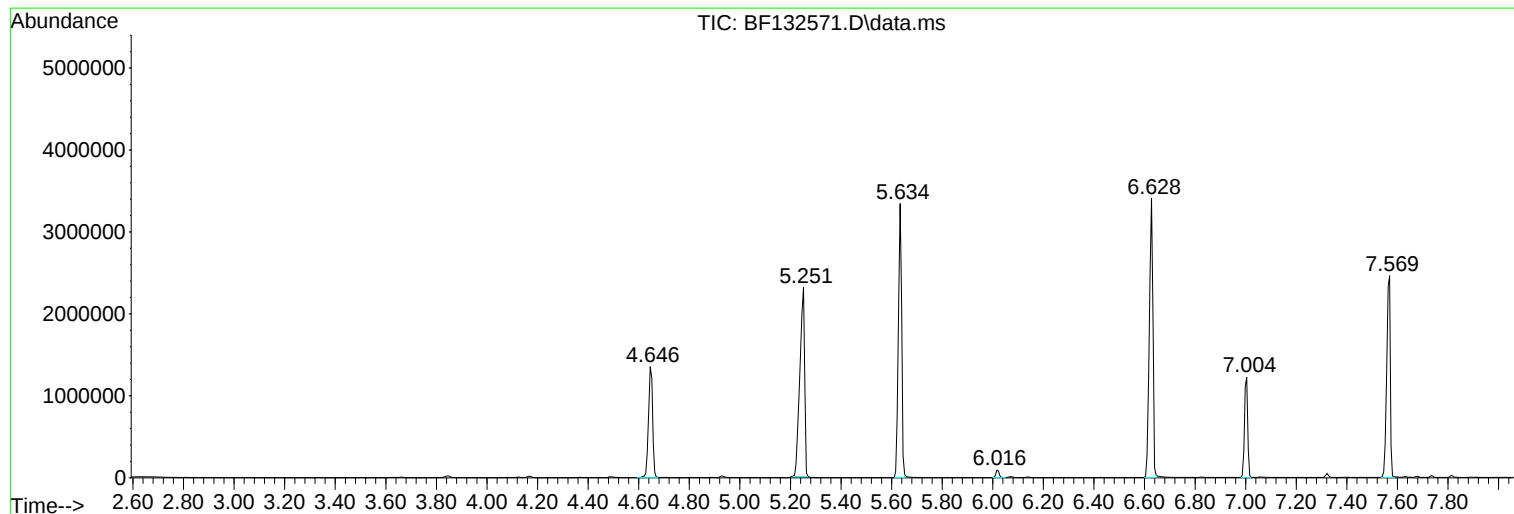

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132571.D
Acq On : 28 Feb 2023 14:40
Operator : CG\JU
Sample : 01703-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KU-CON1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132571.D
Acq On : 28 Feb 2023 14:40
Operator : CG\JU
Sample : 01703-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KU-CON1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------