

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
 Data File : BF132573.D
 Acq On : 28 Feb 2023 15:44
 Operator : CG\JU
 Sample : 01723-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HH-CON-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.646	346	350	357	rBV	446891	454982	7.99%	1.240%
2	5.246	446	452	455	rBV	1924610	2404658	42.24%	6.555%
3	5.634	513	518	521	rBV	3119600	2852665	50.11%	7.776%
4	6.016	580	583	590	rBV	92199	81896	1.44%	0.223%
5	6.628	682	687	690	rBV	3134499	2989360	52.51%	8.149%
6	7.004	747	751	754	rBV	1226118	1108582	19.47%	3.022%
7	7.563	841	846	849	rBV	2208894	2093974	36.78%	5.708%
8	8.287	965	969	972	rBV	1755789	1400793	24.61%	3.818%
9	9.363	1146	1152	1155	rBV	5844339	5105682	89.69%	13.917%
10	10.051	1265	1269	1272	rBV	2596586	2317666	40.71%	6.318%
11	10.763	1386	1390	1393	rBV	757269	607491	10.67%	1.656%
12	10.839	1399	1403	1407	rBV	3007937	2894565	50.85%	7.890%
13	11.545	1519	1523	1526	rBV	2783424	2405317	42.25%	6.557%
14	11.604	1530	1533	1536	rVB2	71221	59264	1.04%	0.162%
15	12.051	1606	1609	1614	rBV	131413	138487	2.43%	0.377%
16	13.133	1789	1793	1797	rBV	5480585	5692748	100.00%	15.518%
17	14.027	1941	1945	1959	rBV2	220920	482410	8.47%	1.315%
18	14.204	1970	1975	1978	rBV	2054655	2041317	35.86%	5.564%
19	15.751	2233	2238	2250	rBV	1086119	1554010	27.30%	4.236%




Sum of corrected areas: 36685867

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132573.D
Acq On : 28 Feb 2023 15:44
Operator : CG\JU
Sample : 01723-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

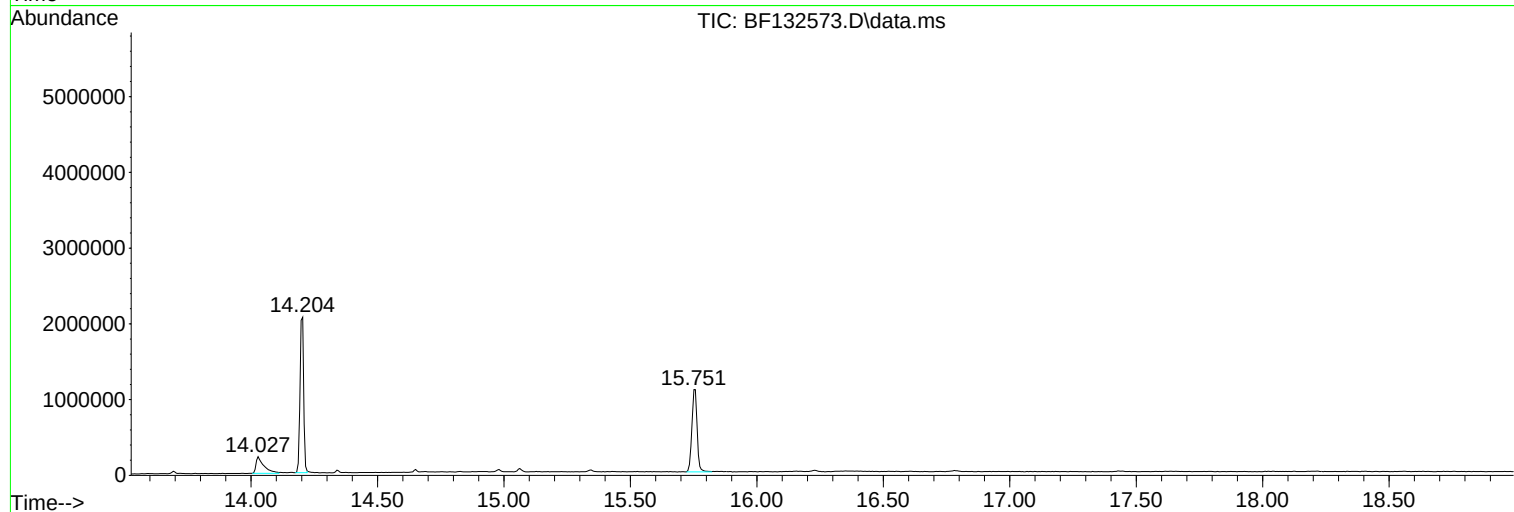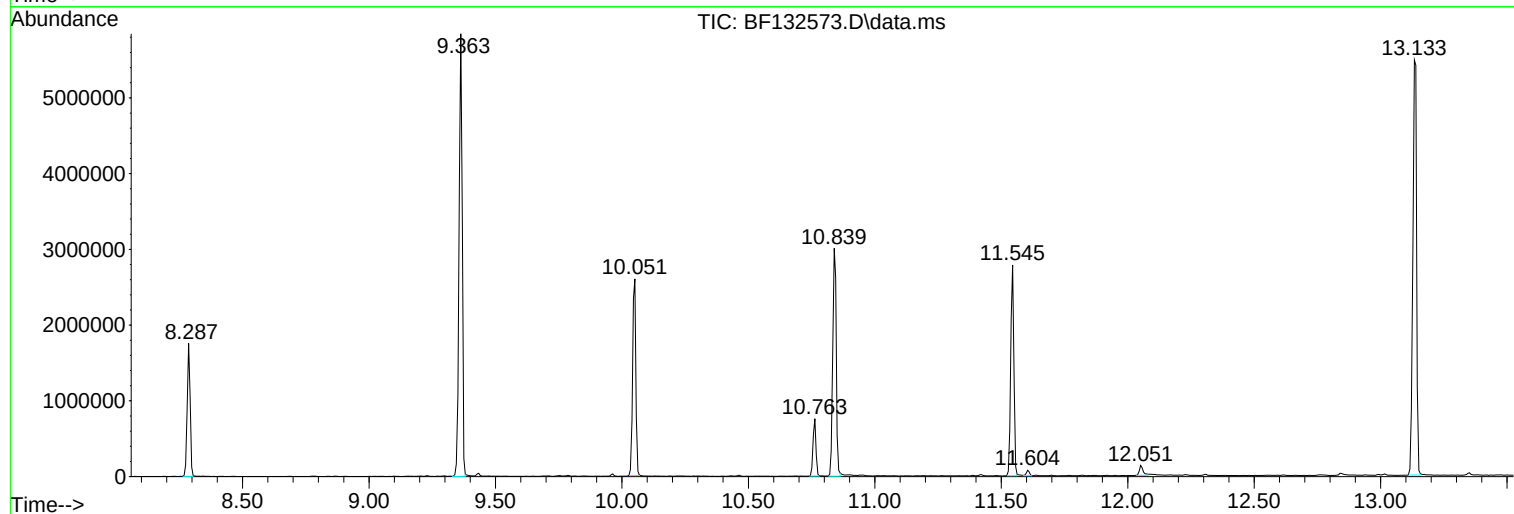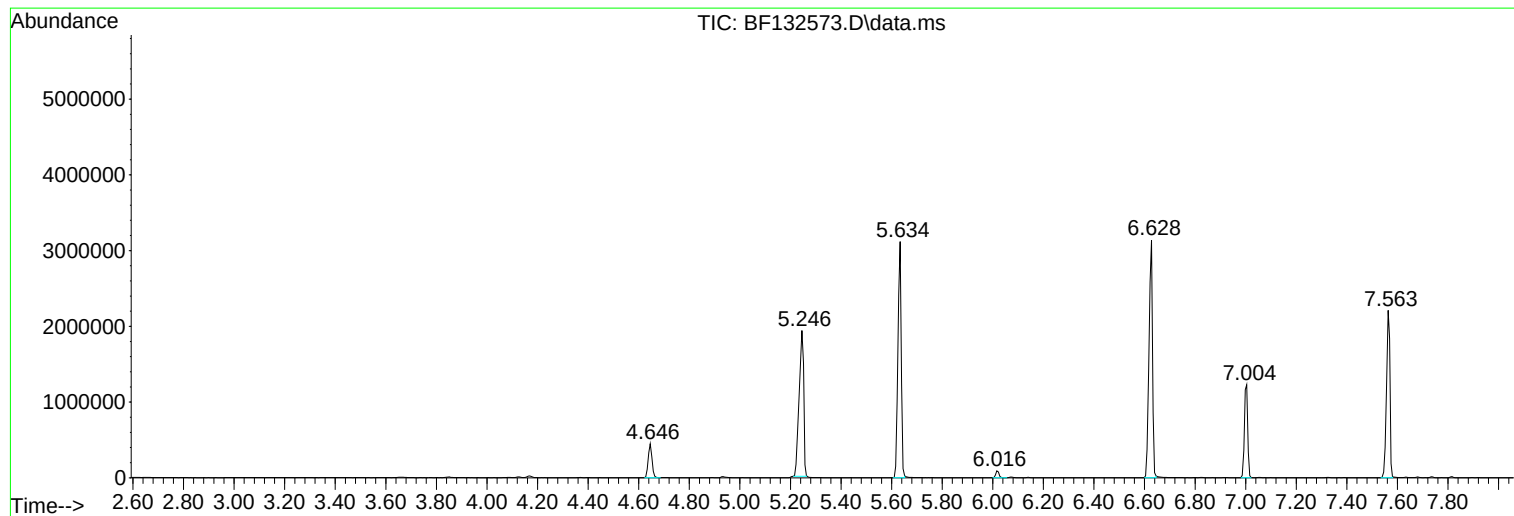

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132573.D
Acq On : 28 Feb 2023 15:44
Operator : CG\JU
Sample : 01723-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132573.D
Acq On : 28 Feb 2023 15:44
Operator : CG\JU
Sample : 01723-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------