

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
 Data File : BF132574.D
 Acq On : 28 Feb 2023 16:16
 Operator : CG\JU
 Sample : 01723-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HH-CON-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.646	346	350	358	rBV	681541	726299	12.81%	1.828%
2	5.251	446	453	456	rVB	2489849	3301083	58.22%	8.306%
3	5.634	513	518	521	rBV	3881261	3521552	62.11%	8.861%
4	6.016	580	583	589	rBV	128454	110257	1.94%	0.277%
5	6.628	682	687	690	rBV	3975711	3996143	70.48%	10.055%
6	6.998	747	750	754	rBV	1650573	1452191	25.61%	3.654%
7	7.563	841	846	849	rBV	2831755	2723712	48.04%	6.854%
8	8.287	965	969	972	rBV	2234450	1850370	32.63%	4.656%
9	9.363	1146	1152	1155	rBV	5713532	4938067	87.09%	12.426%
10	10.051	1265	1269	1272	rBV	2489066	2157521	38.05%	5.429%
11	10.763	1386	1390	1393	rBV	664352	543297	9.58%	1.367%
12	10.839	1399	1403	1413	rBV	2652961	2368568	41.77%	5.960%
13	11.545	1519	1523	1526	rBV	2701508	2371784	41.83%	5.968%
14	12.051	1606	1609	1622	rVB2	135203	152694	2.69%	0.384%
15	13.133	1789	1793	1797	rBV	5424093	5670065	100.00%	14.267%
16	14.027	1941	1945	1965	rBV2	225506	511605	9.02%	1.287%
17	14.198	1970	1974	1978	rBV	2064061	1940171	34.22%	4.882%
18	15.751	2232	2238	2246	rBV2	1039570	1405978	24.80%	3.538%




Sum of corrected areas: 39741357

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132574.D
Acq On : 28 Feb 2023 16:16
Operator : CG\JU
Sample : 01723-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

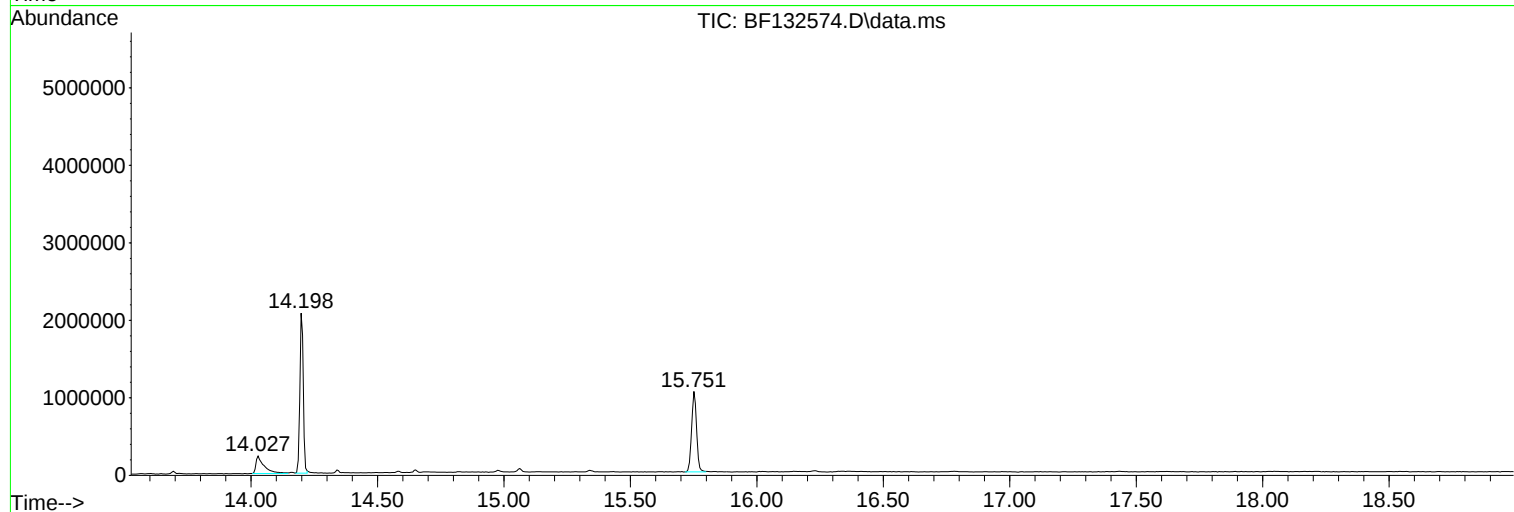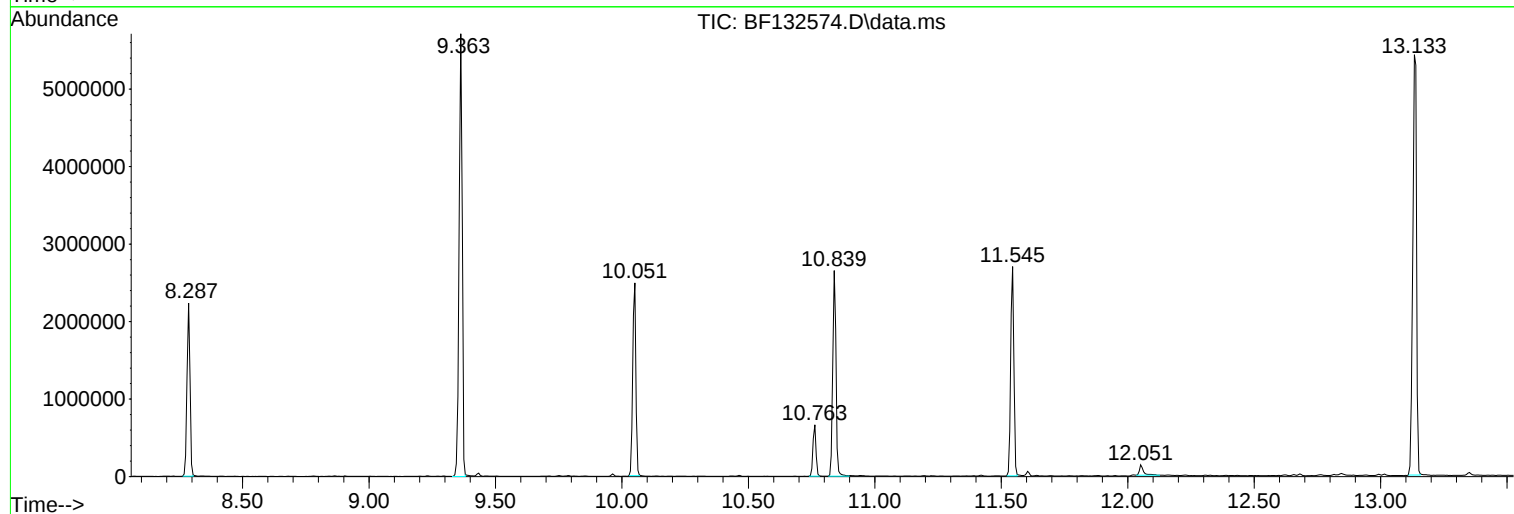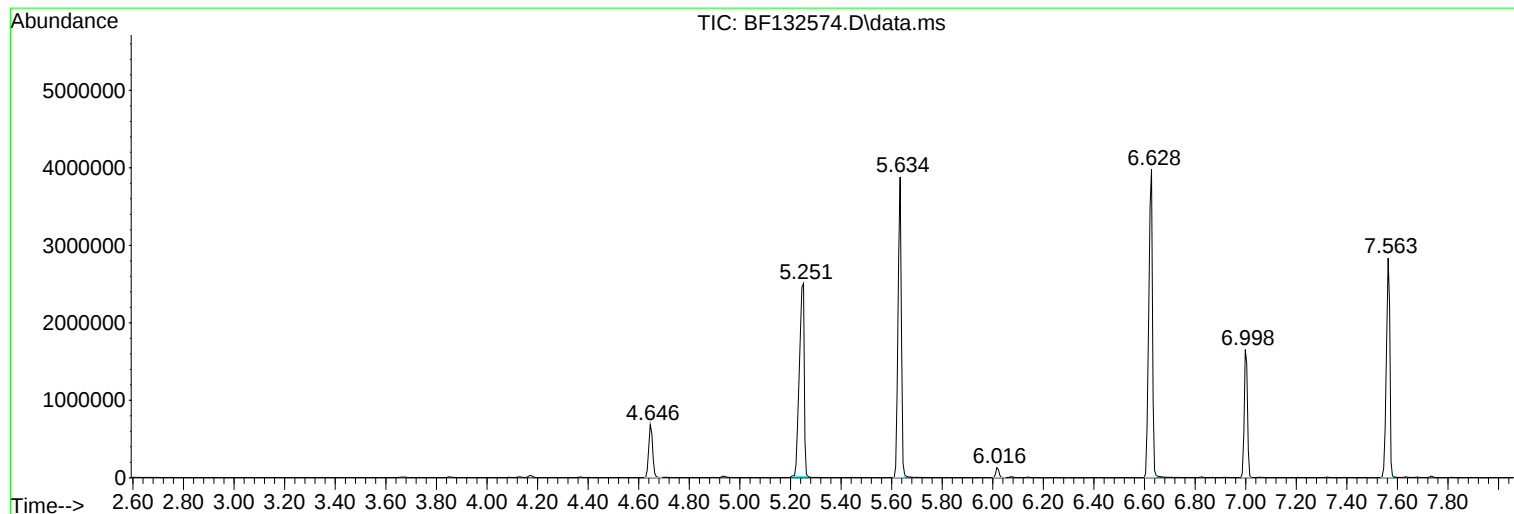

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132574.D
Acq On : 28 Feb 2023 16:16
Operator : CG\JU
Sample : 01723-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132574.D
Acq On : 28 Feb 2023 16:16
Operator : CG\JU
Sample : 01723-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------