

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
 Data File : BF132575.D
 Acq On : 28 Feb 2023 16:48
 Operator : CG\JU
 Sample : 01723-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HH-CON-4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.646	346	350	356	rBV	687073	718440	13.35%	1.517%
2	5.251	446	453	456	rVB	3162319	4568302	84.91%	9.649%
3	5.604	510	513	514	rBV	214604	176140	3.27%	0.372%
4	5.628	514	517	521	rVB	2959105	2871656	53.37%	6.065%
5	5.799	543	546	550	rBV	291216	259191	4.82%	0.547%
6	5.857	553	556	560	rVB	244018	229228	4.26%	0.484%
7	6.016	580	583	590	rBV	135127	113823	2.12%	0.240%
8	6.463	656	659	662	rBV	117547	99926	1.86%	0.211%
9	6.528	666	670	672	rBV	469741	428366	7.96%	0.905%
10	6.557	672	675	678	rVV	140059	110000	2.04%	0.232%
11	6.598	679	682	683	rVV	621446	492075	9.15%	1.039%
12	6.628	683	687	690	rVV	3596133	3682884	68.45%	7.779%
13	6.687	693	697	700	rVV	439346	363721	6.76%	0.768%
14	6.751	702	708	711	rBV	117602	123066	2.29%	0.260%
15	6.822	717	720	724	rVB	1298938	1093751	20.33%	2.310%
16	6.998	747	750	753	rBV	1599852	1471429	27.35%	3.108%
17	7.022	753	754	757	rVB	74290	53845	1.00%	0.114%
18	7.057	757	760	763	rBV2	458397	441049	8.20%	0.932%
19	7.104	763	768	775	rVB2	198136	355893	6.61%	0.752%
20	7.157	775	777	779	rBV	78438	71833	1.34%	0.152%
21	7.269	794	796	800	rVB	105644	82809	1.54%	0.175%
22	7.316	800	804	807	rBV	166597	156133	2.90%	0.330%
23	7.404	814	819	822	rVB2	53804	72647	1.35%	0.153%
24	7.563	842	846	849	rVB	2916015	2662163	49.48%	5.623%
25	7.698	867	869	873	rVB	123748	102582	1.91%	0.217%
26	7.892	898	902	908	rVB	114156	90148	1.68%	0.190%
27	7.963	908	914	916	rBV	77109	71004	1.32%	0.150%
28	7.992	916	919	920	rVV	147985	122038	2.27%	0.258%
29	8.010	920	922	926	rVB2	139995	135286	2.51%	0.286%
30	8.204	953	955	960	rVB2	70430	63409	1.18%	0.134%
31	8.287	965	969	972	rBV	2275695	1801493	33.48%	3.805%
32	9.363	1146	1152	1155	rBV	5557421	4944573	91.90%	10.444%
33	9.963	1248	1254	1257	rBV	84073	69320	1.29%	0.146%
34	10.051	1265	1269	1272	rBV	2473056	2146461	39.89%	4.534%
35	10.463	1336	1339	1342	rVB	105209	83158	1.55%	0.176%
36	10.763	1386	1390	1393	rVB	612599	526851	9.79%	1.113%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
 Data File : BF132575.D
 Acq On : 28 Feb 2023 16:48
 Operator : CG\JU
 Sample : 01723-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HH-CON-4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	10.839	1399	1403	1414	rBV	2039375	1763682	32.78%	3.725%
38	10.939	1417	1420	1424	rBV	102847	107717	2.00%	0.228%
39	11.545	1519	1523	1526	rBV	2693167	2281276	42.40%	4.818%
40	12.051	1606	1609	1622	rBV2	201711	275843	5.13%	0.583%
41	12.304	1647	1652	1658	rBV3	90651	110984	2.06%	0.234%
42	12.492	1679	1684	1690	rVB6	50756	87896	1.63%	0.186%
43	12.657	1708	1712	1717	rBV	147507	185406	3.45%	0.392%
44	12.727	1717	1724	1726	rBV	184151	238050	4.42%	0.503%
45	12.816	1737	1739	1741	rVB	75462	55415	1.03%	0.117%
46	13.033	1774	1776	1780	rVB3	66342	60332	1.12%	0.127%
47	13.133	1789	1793	1797	rVB	5424056	5380341	100.00%	11.364%
48	13.251	1810	1813	1819	rVB	53897	55967	1.04%	0.118%
49	13.351	1826	1830	1832	rBV	68564	65066	1.21%	0.137%
50	13.533	1857	1861	1864	rBV2	46268	63730	1.18%	0.135%
51	13.604	1870	1873	1876	rVB	64713	62902	1.17%	0.133%
52	13.692	1883	1888	1890	rBV3	105196	126013	2.34%	0.266%
53	13.733	1893	1895	1898	rVB	147361	124585	2.32%	0.263%
54	13.833	1909	1912	1915	rBV	92583	89131	1.66%	0.188%
55	13.874	1915	1919	1922	rVB	289742	252361	4.69%	0.533%
56	14.022	1941	1944	1961	rVB	332323	601862	11.19%	1.271%
57	14.198	1970	1974	1978	rBV	1843429	1721535	32.00%	3.636%
58	14.339	1995	1998	2000	rBV	72926	64986	1.21%	0.137%
59	14.427	2009	2013	2017	rBV	91215	103022	1.91%	0.218%
60	14.580	2035	2039	2043	rBV	1094132	968690	18.00%	2.046%
61	14.651	2047	2051	2054	rVV	82570	80261	1.49%	0.170%
62	14.980	2103	2107	2109	rBV	48723	57771	1.07%	0.122%
63	15.063	2118	2121	2124	rVB	55440	54731	1.02%	0.116%
64	15.339	2165	2168	2176	rVB	43900	58539	1.09%	0.124%
65	15.751	2233	2238	2252	rVB	966257	1318427	24.50%	2.785%
66	16.051	2285	2289	2294	rVB8	48845	73122	1.36%	0.154%




Sum of corrected areas: 47344336

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132575.D
Acq On : 28 Feb 2023 16:48
Operator : CG\JU
Sample : 01723-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

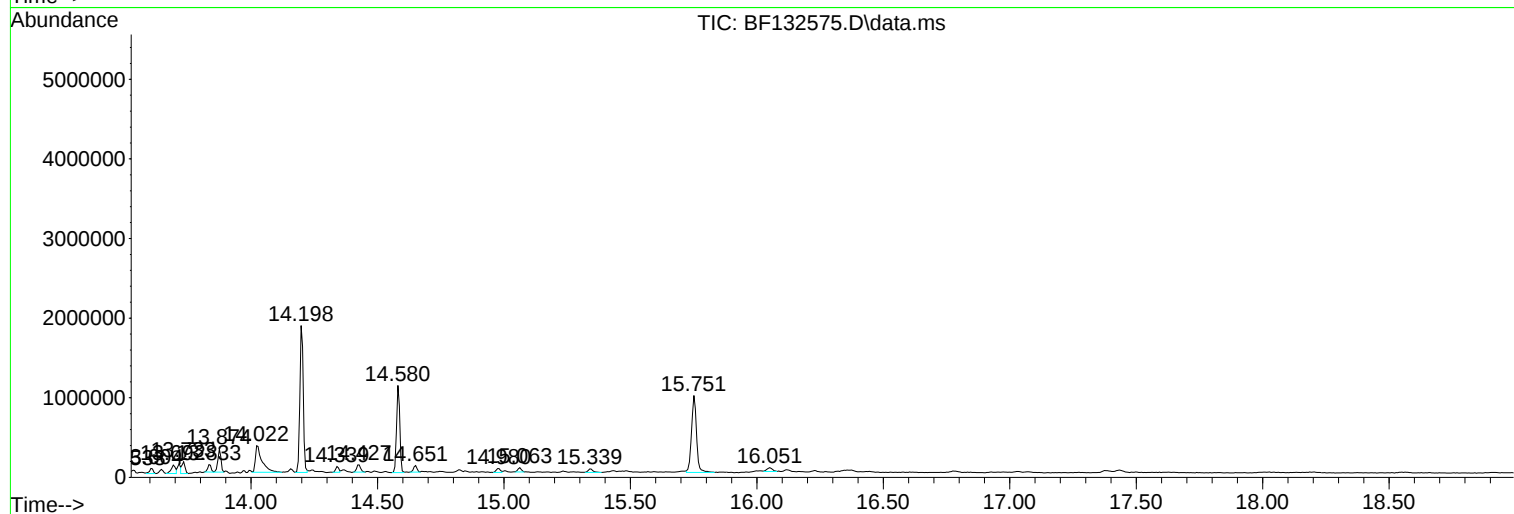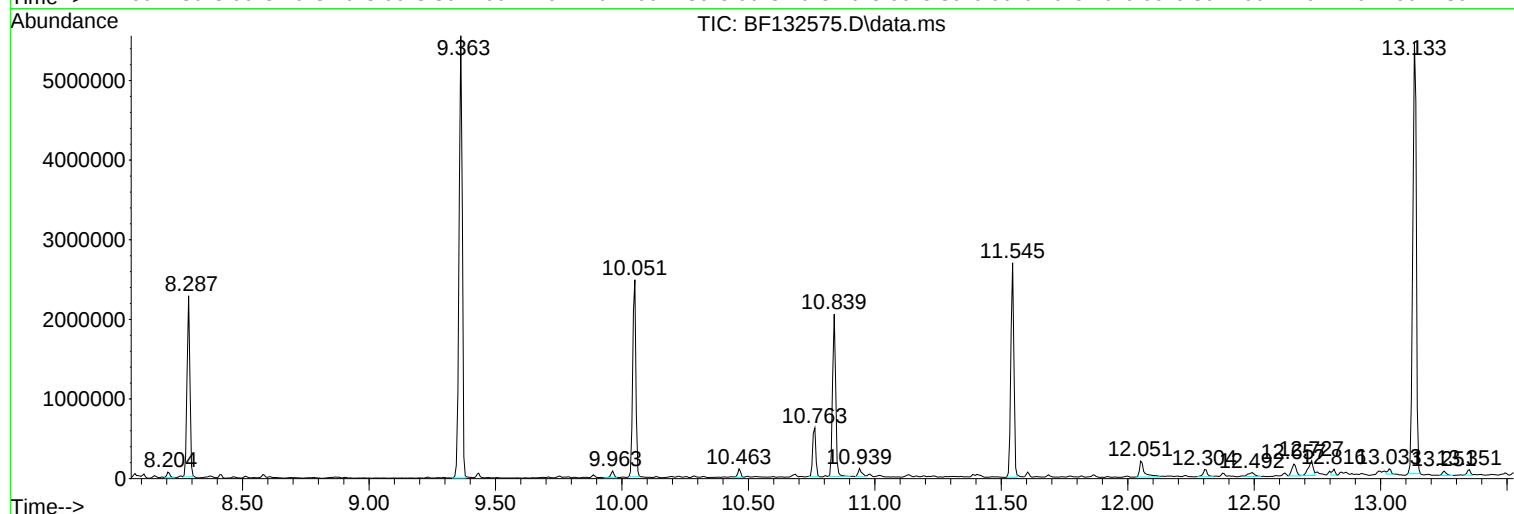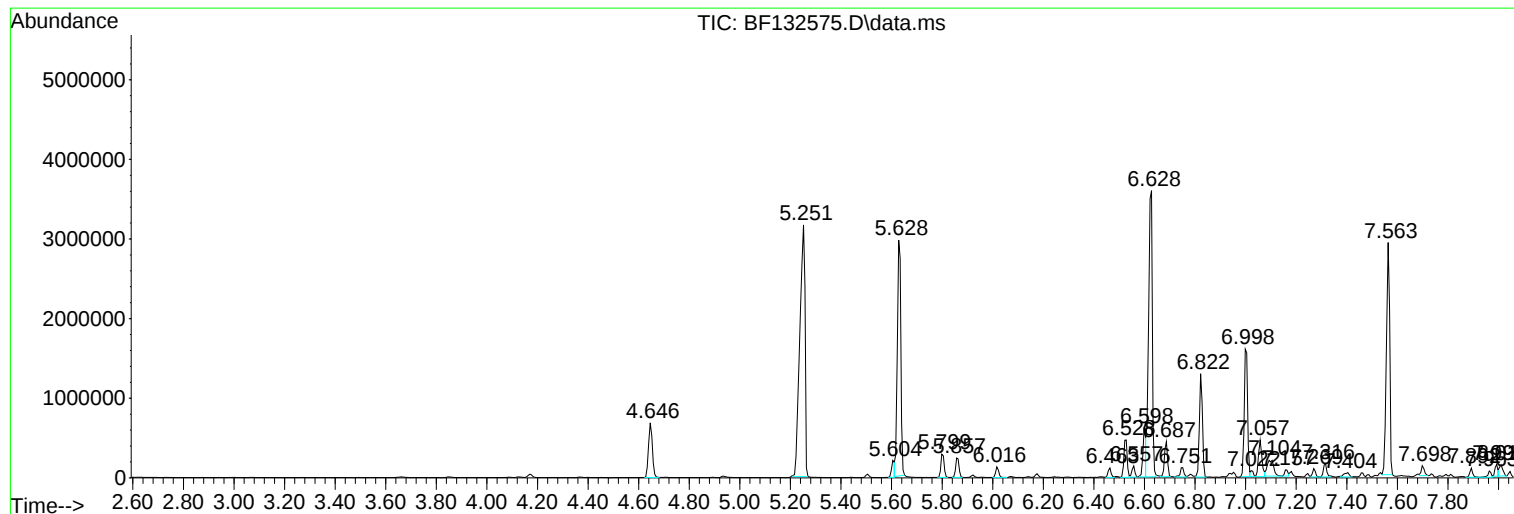

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132575.D
Acq On : 28 Feb 2023 16:48
Operator : CG\JU
Sample : 01723-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132575.D
Acq On : 28 Feb 2023 16:48
Operator : CG\JU
Sample : 01723-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HH-CON-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------