


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132564.D
Acq On : 28 Feb 2023 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 24 23:17:30 2023

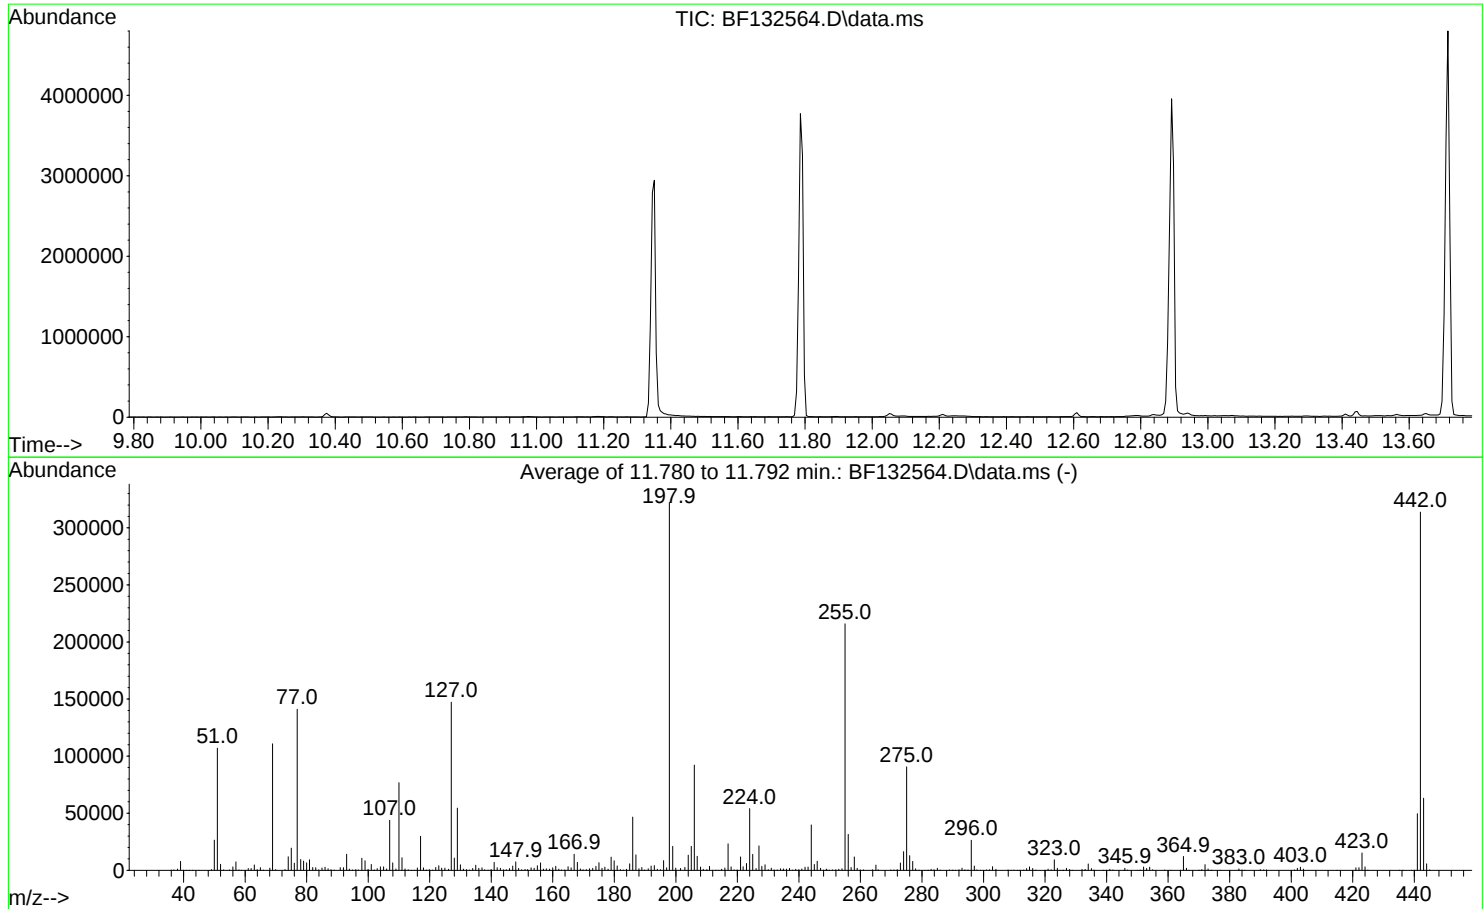




AutoFind: Scans 1563, 1564, 1565; Background Corrected with Scan 1558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	107037	PASS
68	69	0.00	2	1.7	1863	PASS
69	198	0.00	100	34.4	110836	PASS
70	69	0.00	2	0.6	672	PASS
127	198	10	80	45.7	147341	PASS
197	198	0.00	2	0.7	2255	PASS
198	198	100	100	100.0	322283	PASS
199	198	5	9	6.5	20961	PASS
275	198	10	60	28.1	90651	PASS
365	198	1	100	3.8	12153	PASS
441	198	0.01	100	15.4	49628	PASS
442	442	50	100	100.0	313811	PASS
443	442	15	24	20.1	63091	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132564.D
Acq On : 28 Feb 2023 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 01 04:27:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

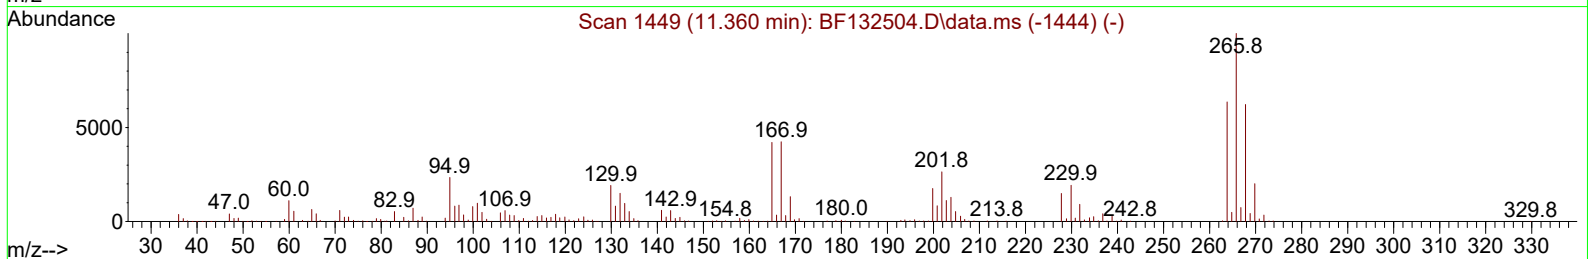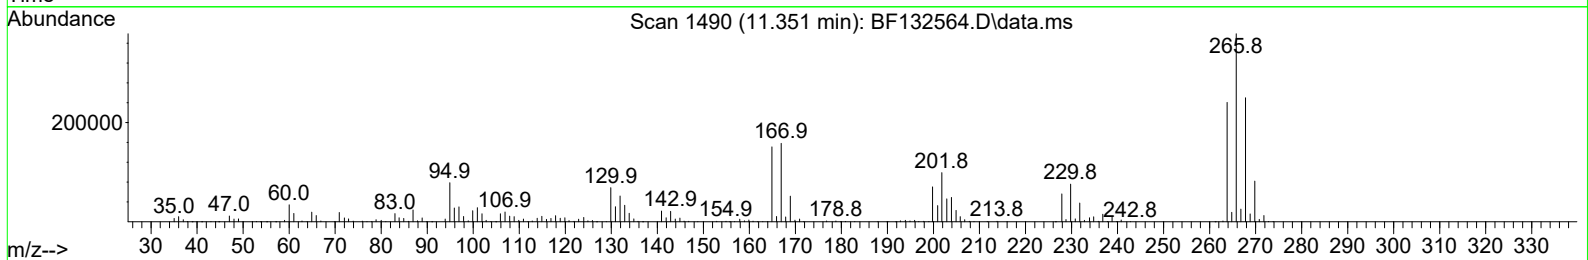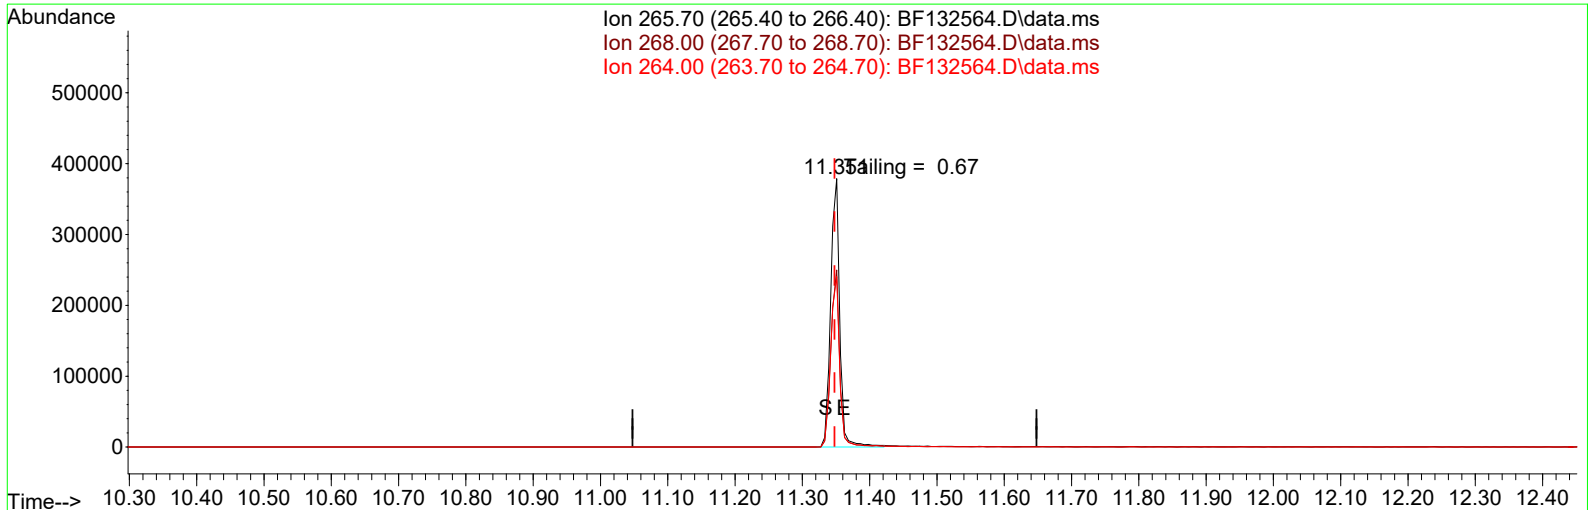

TIC: BF132564.D\data.ms

(70) Pentachlorophenol (C)

11.351min (+ 0.003) 857385.03 ng




response 358223

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.96
264.00	63.60	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022823\
Data File : BF132564.D
Acq On : 28 Feb 2023 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 01 04:27:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

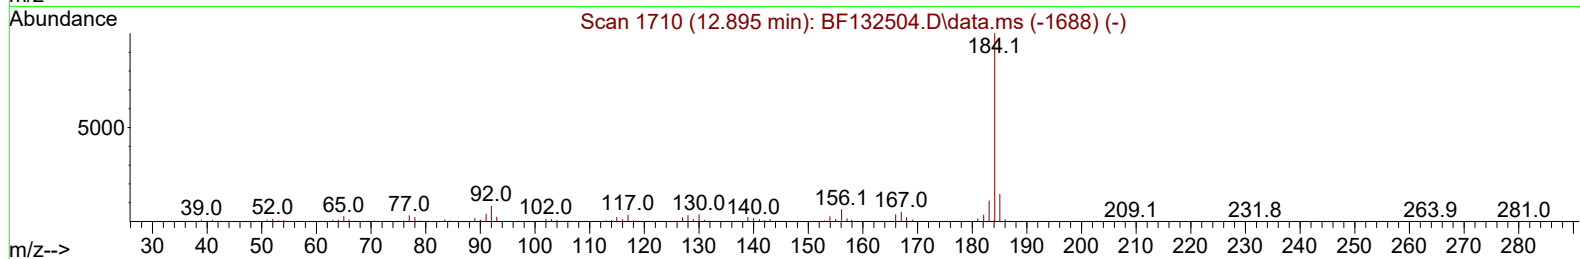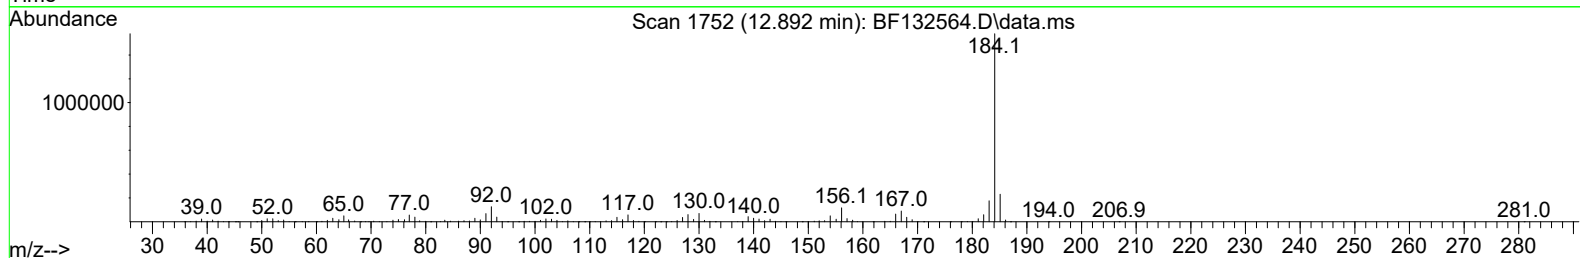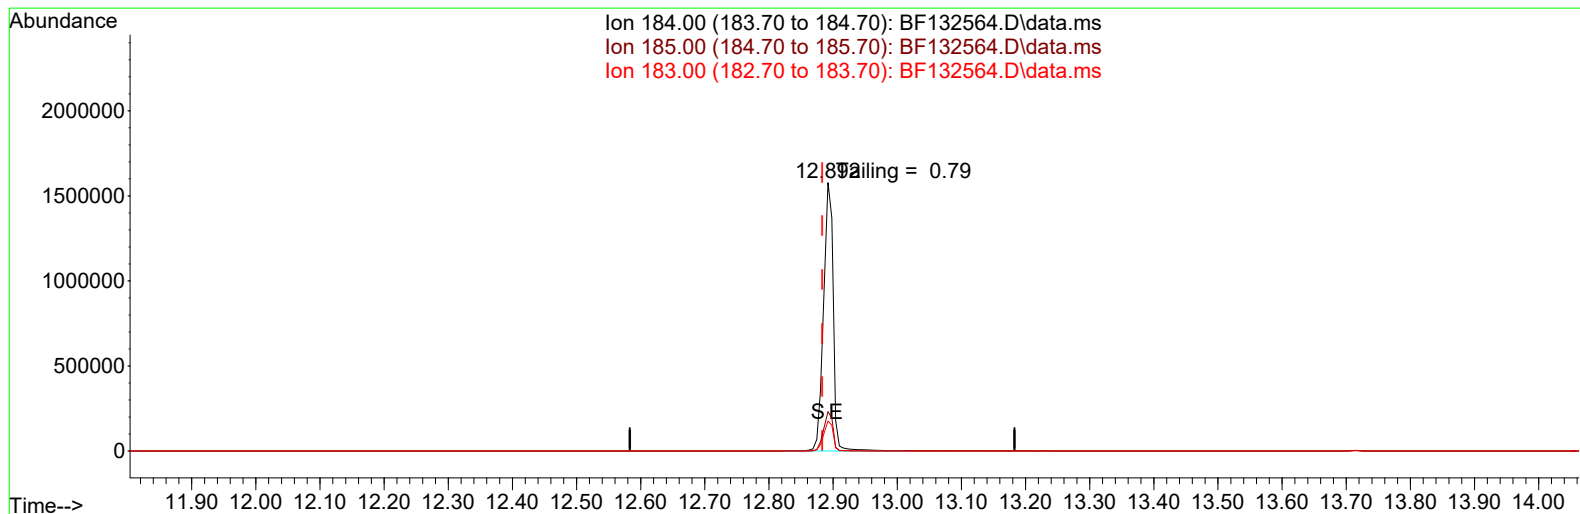

TIC: BF132564.D\data.ms

(77) Benzidine

12.892min (+ 0.009) 1053622.00 ng

response 1667131

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.66
183.00	10.90	11.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/28/2023	BNA_F	<u>BF132564.D</u>
Compound Name	Response	Retention Time
DDT	874576	13.715
DDD	15158	13.445
DDE	1858	13.074
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17016	891592	1.91

Instrument :
BNA_F
ClientSampleId :
DFTPP