


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030119\
 Data File : BF112790.D
 Acq On : 1 Mar 2019 10:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 15:40:43 2019

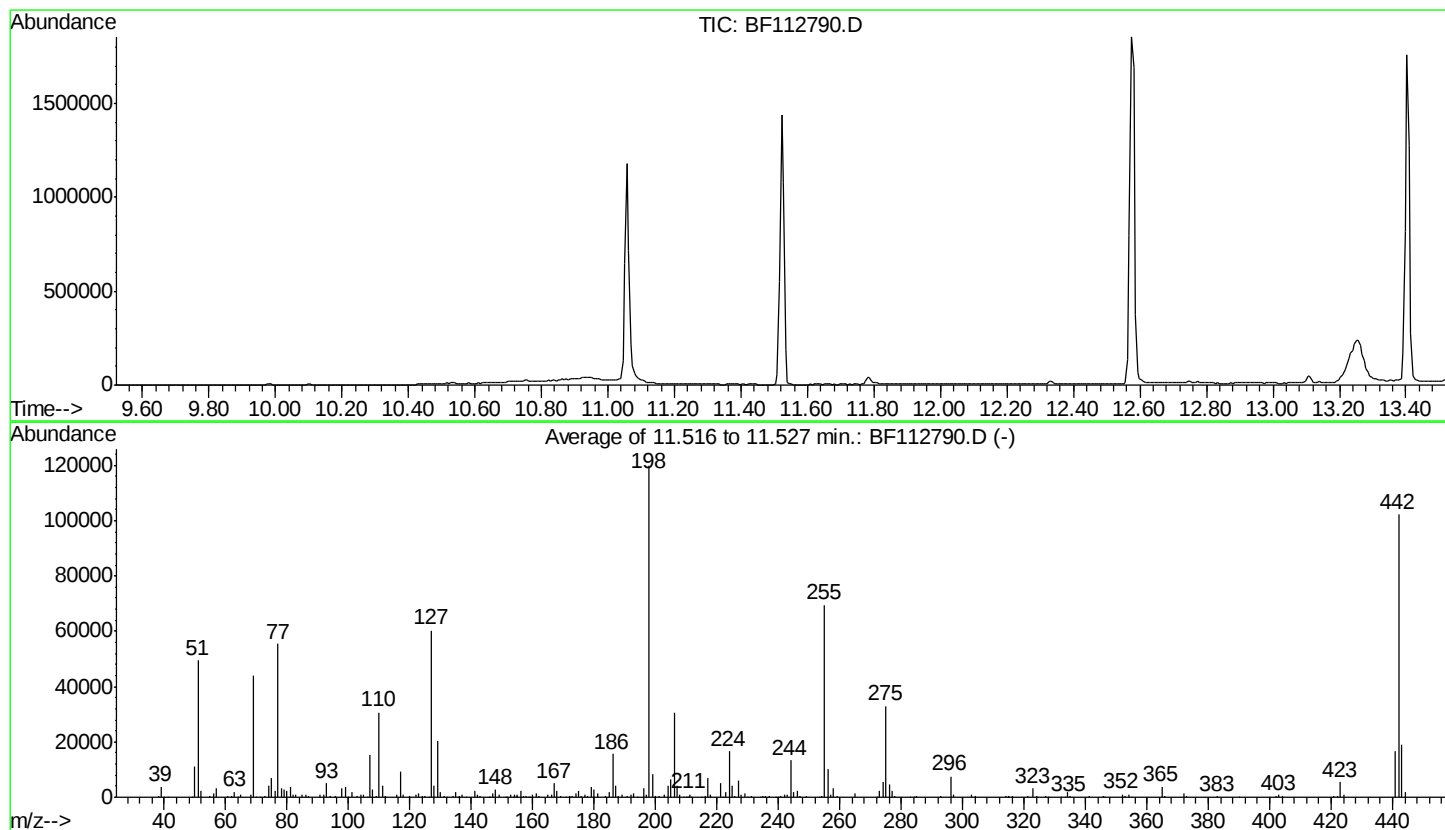

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	49504	PASS
68	69	0.00	2	1.7	761	PASS
69	198	0.00	100	36.8	44117	PASS
70	69	0.00	2	0.5	211	PASS
127	198	10	80	50.4	60386	PASS
197	198	0.00	2	0.7	833	PASS
198	198	100	100	100.0	119877	PASS
199	198	5	9	6.9	8321	PASS
275	198	10	60	27.5	33010	PASS
365	198	1	100	3.1	3771	PASS
441	198	0.01	100	13.8	16484	PASS
442	198	50	100	85.2	102149	PASS
443	442	15	24	18.6	19013	PASS