


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030123\
Data File : BF132583.D
Acq On : 01 Mar 2023 10:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 24 23:17:30 2023

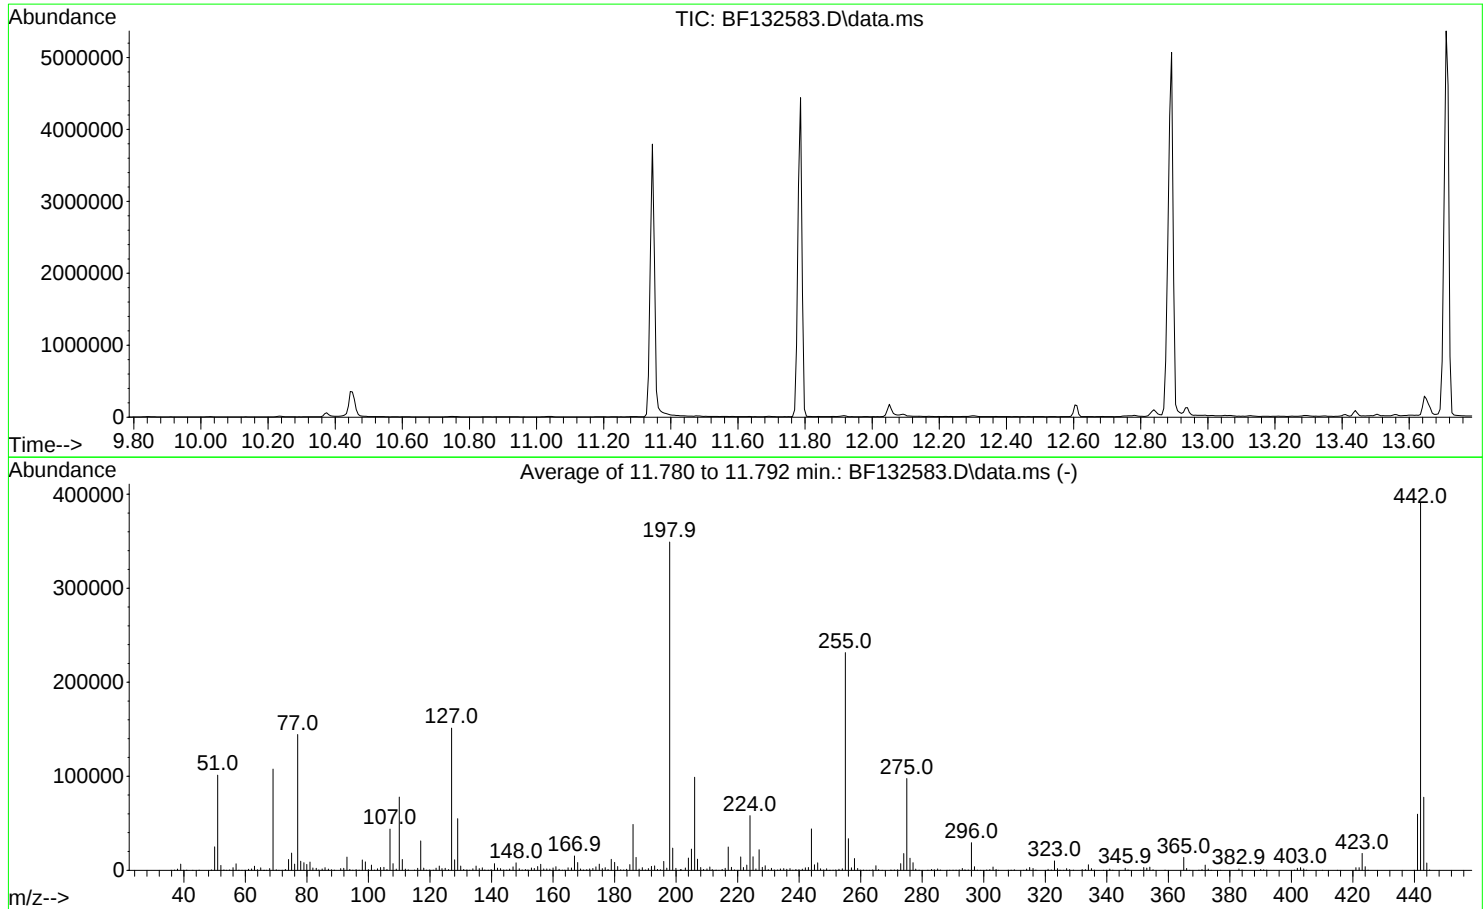




AutoFind: Scans 1563, 1564, 1565; Background Corrected with Scan 1557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	101253	PASS
68	69	0.00	2	1.7	1844	PASS
69	198	0.00	100	30.8	107693	PASS
70	69	0.00	2	0.6	681	PASS
127	198	10	80	43.3	151288	PASS
197	198	0.00	2	0.6	2251	PASS
198	198	100	100	100.0	349163	PASS
199	198	5	9	6.8	23612	PASS
275	198	10	60	27.9	97536	PASS
365	198	1	100	3.9	13769	PASS
441	198	0.01	100	17.1	59624	PASS
442	442	50	100	100.0	391253	PASS
443	442	15	24	19.8	77635	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030123\
Data File : BF132583.D
Acq On : 01 Mar 2023 10:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 02 06:07:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

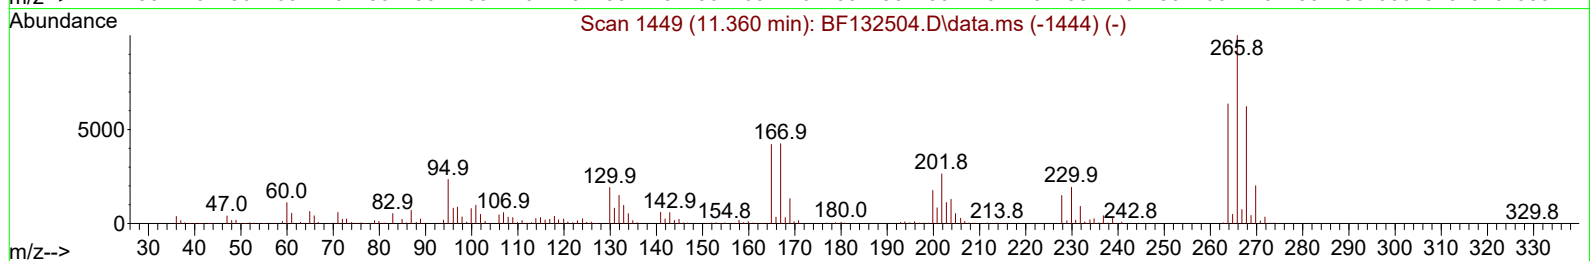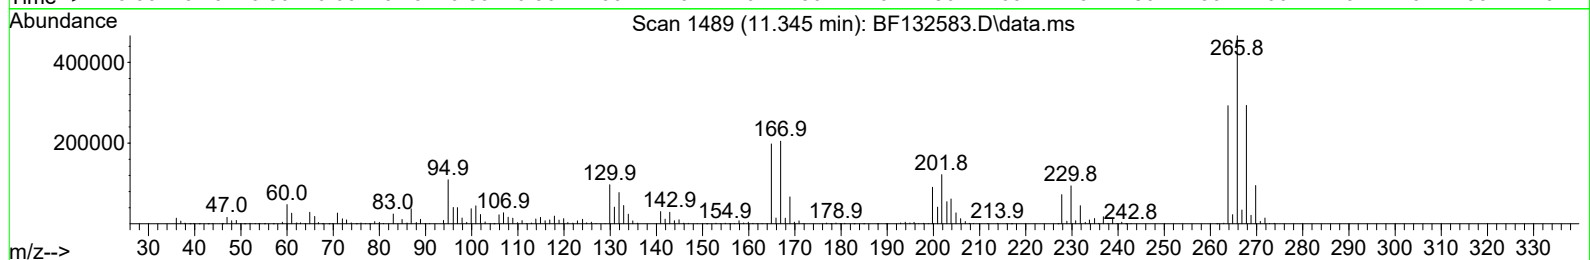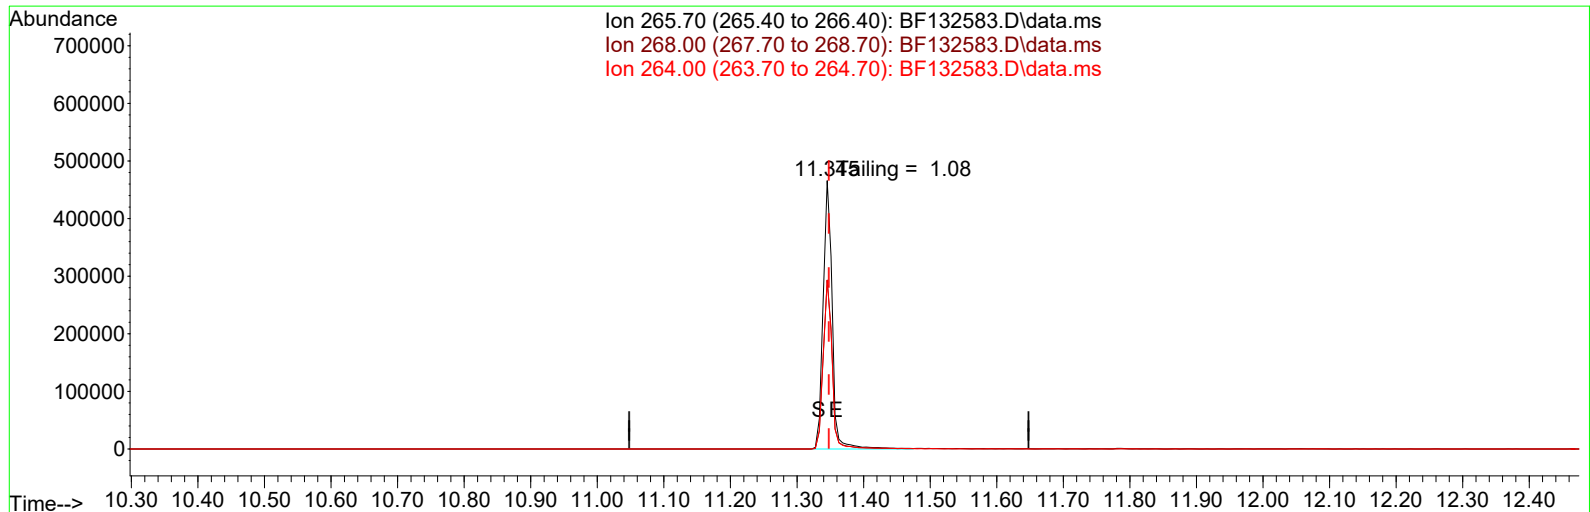

TIC: BF132583.D\data.ms

(70) Pentachlorophenol (C)

11.345min (-0.003) 595836.49 ng




response 443039

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.99
264.00	63.60	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030123\
 Data File : BF132583.D
 Acq On : 01 Mar 2023 10:50
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 02 06:07:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 23:17:30 2023
 Response via : Initial Calibration

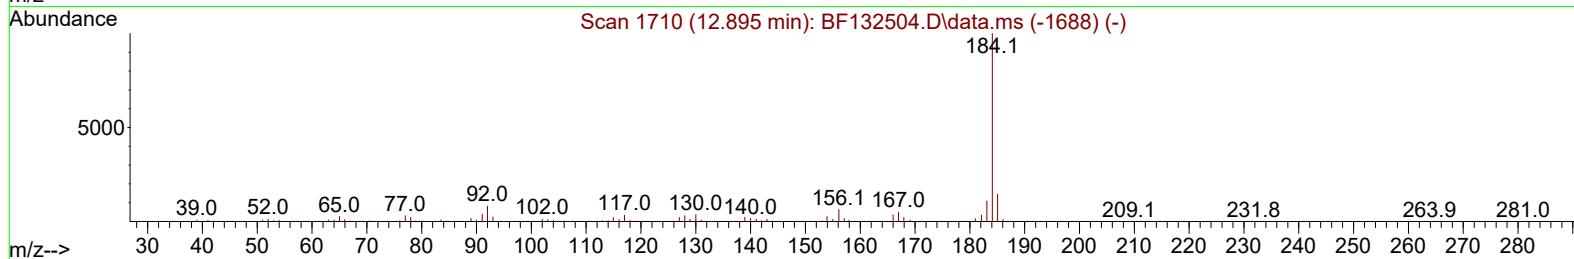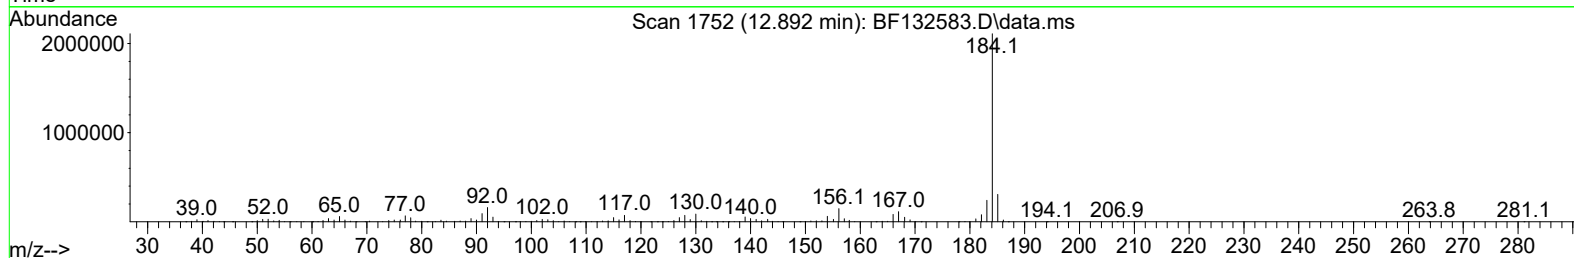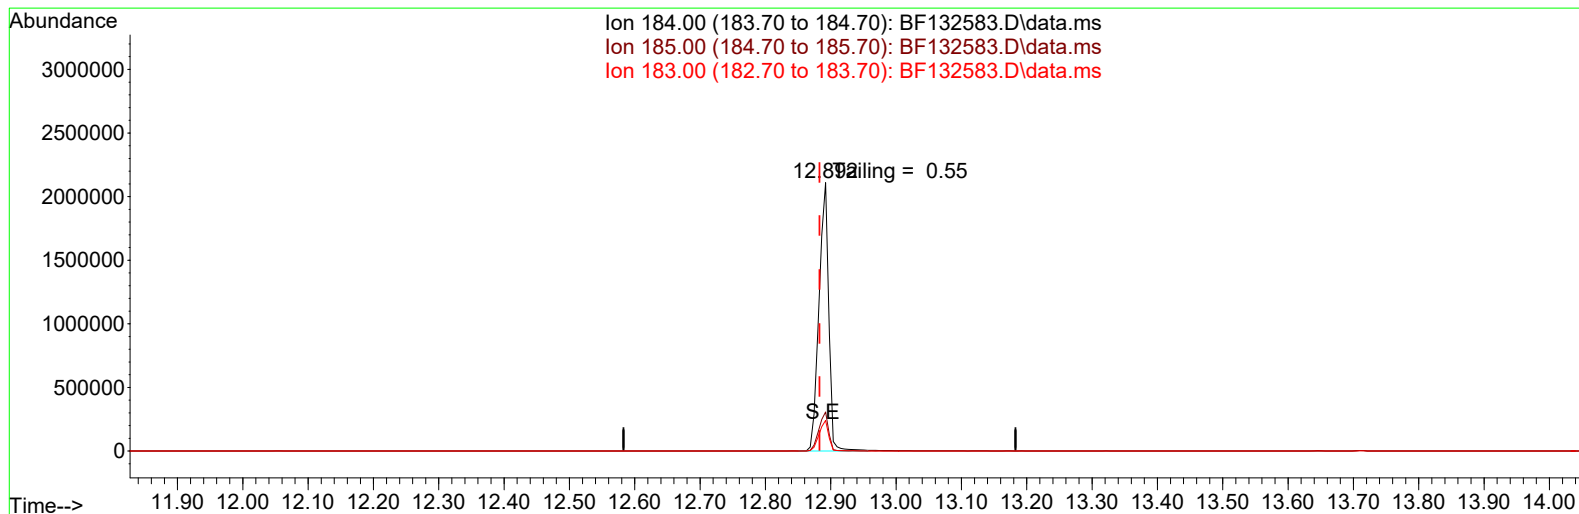

TIC: BF132583.D\data.ms

(77) Benzidine

12.892min (+ 0.009) 147312.54 ng

response 2205395

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.54
183.00	10.90	11.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/1/2023	BNA_F	<u>BF132583.D</u>
Compound Name	Response	Retention Time
DDT	1076644	13.71
DDD	17429	13.439
DDE	1467	13.069
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18896	1095540	1.72

Instrument :
BNA_F
ClientSampleId :
DFTPP