
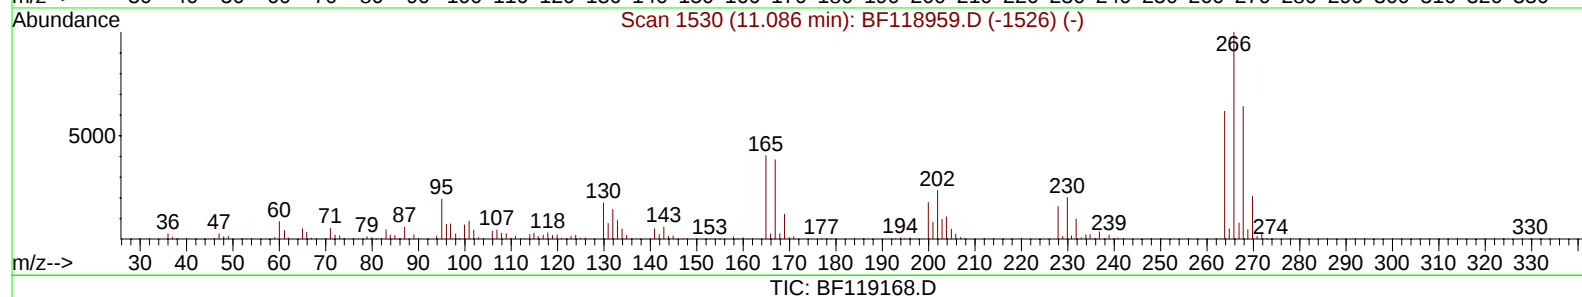
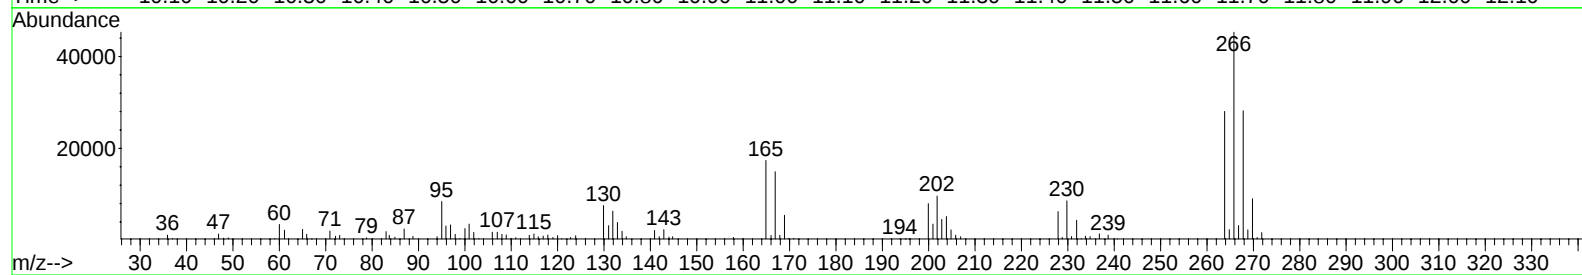


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF030220\
 Data File : BF119168.D
 Acq On : 2 Mar 2020 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 19:17:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 26 16:03:05 2020
 Response via : Initial Calibration

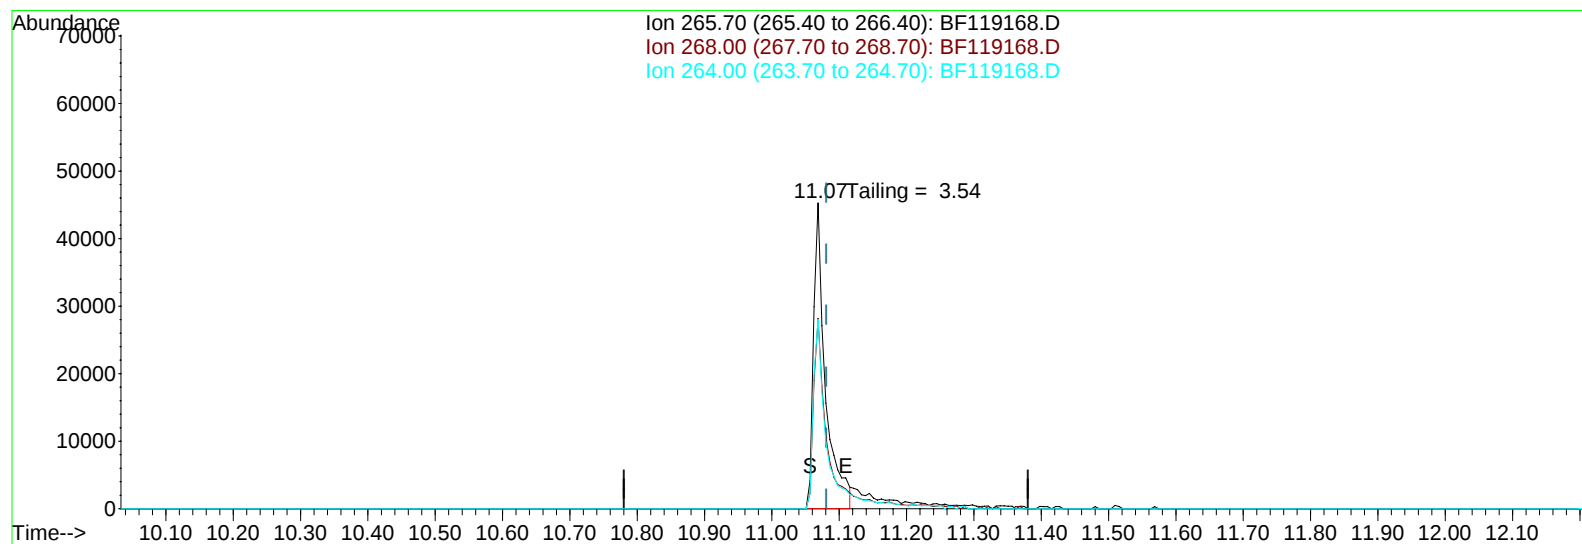

TIC: BF119168.D

(70) Pentachlorophenol (C)




11.069min (-0.012) 22030.80ng

response 64732

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	62.29
264.00	63.70	61.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF030220\
 Data File : BF119168.D
 Acq On : 2 Mar 2020 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 19:17:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 26 16:03:05 2020
 Response via : Initial Calibration

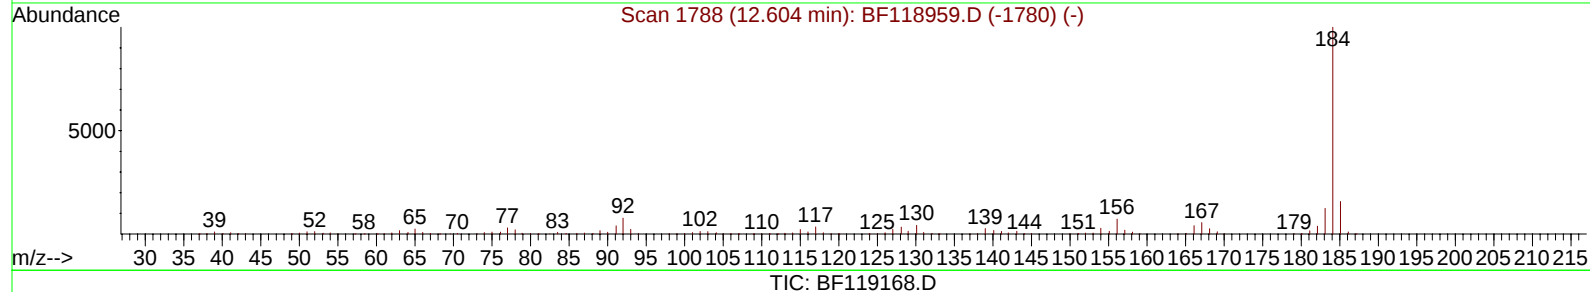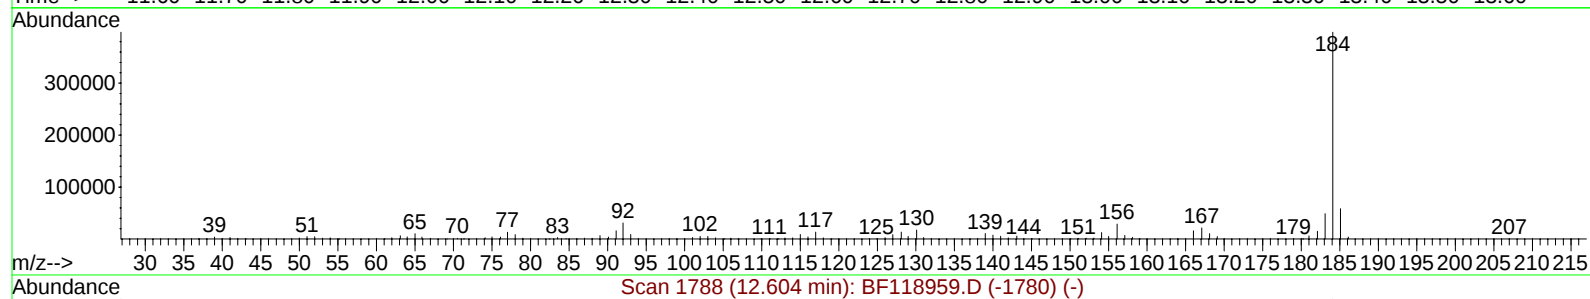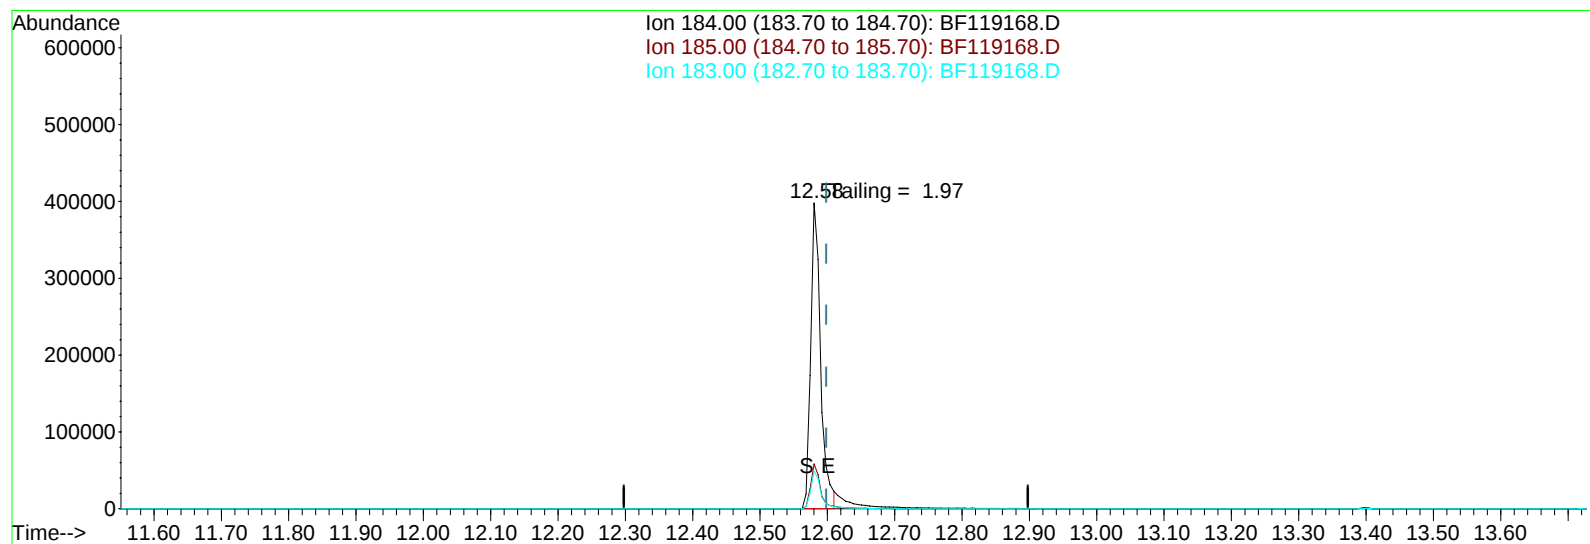

(77) Benzidine

12.580min (-0.018) 0.00ng

response 440821

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.67
183.00	12.40	12.31
0.00	0.00	0.00