

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030221\
 Data File : BF123337.D
 Acq On : 2 Mar 2021 15:39
 Operator : JU/CG
 Sample : M1500-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T-2

Quant Time: Mar 02 17:18:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 16:08:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.851	152	135637	20.00	ng	# 0.00
21) Naphthalene-d8	8.145	136	445475	20.00	ng	# 0.00
39) Acenaphthene-d10	9.910	164	277840	20.00	ng	0.00
64) Phenanthrene-d10	11.398	188	488550	20.00	ng	# 0.00
76) Chrysene-d12	14.039	240	344619	20.00	ng	0.00
86) Perylene-d12	15.515	264	300130	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	805645	85.50	ng	0.00
7) Phenol-d6	6.487	99	1048011	81.86	ng	0.00
23) Nitrobenzene-d5	7.416	82	711759	73.14	ng	-0.01
42) 2,4,6-Tribromophenol	10.704	330	245803	86.88	ng	0.00
45) 2-Fluorobiphenyl	9.222	172	1076555	55.66	ng	0.00
79) Terphenyl-d14	12.986	244	1091510	60.90	ng	0.00
Target Compounds						
						Qvalue
10) Phenol	6.498	94	29906	2.14	ng	86
22) Acetophenone	7.251	105	350006	30.29	ng	# 56
37) 2-Methylnaphthalene	8.857	142	114265	7.03	ng	99
38) 1-Methylnaphthalene	8.957	142	434580	28.57	ng	99
46) 1,1'-Biphenyl	9.322	154	91610	3.97	ng	94
52) Acenaphthene	9.939	154	85847	4.51	ng	# 83
58) Fluorene	10.457	166	176759	8.72	ng	# 90
71) Phenanthrene	11.427	178	555151	19.22	ng	96
78) Pyrene	12.845	202	128418	4.77	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030221\
Data File : BF123337.D
Acq On : 2 Mar 2021 15:39
Operator : JU/CG
Sample : M1500-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T-2

Quant Time: Mar 02 17:18:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration




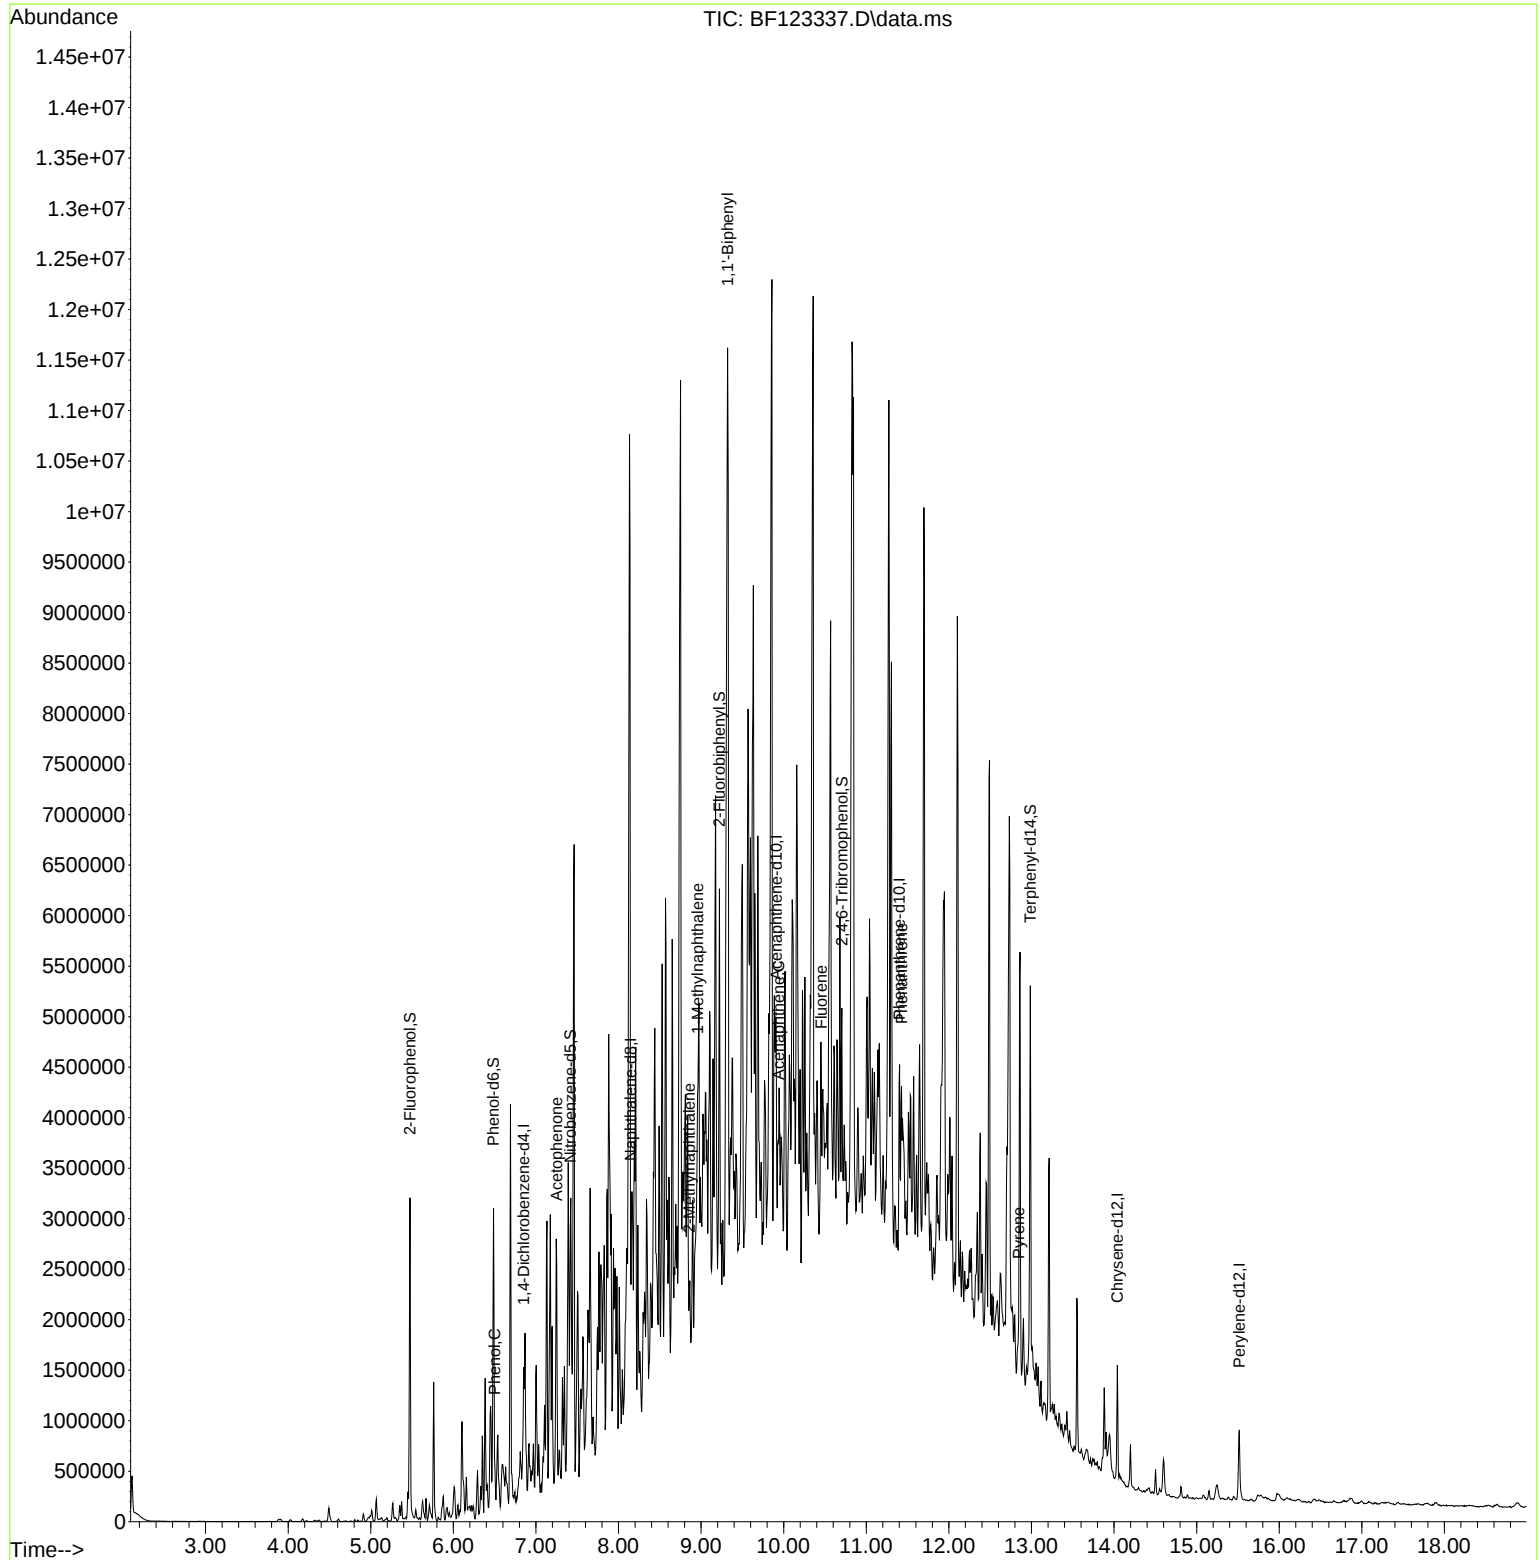


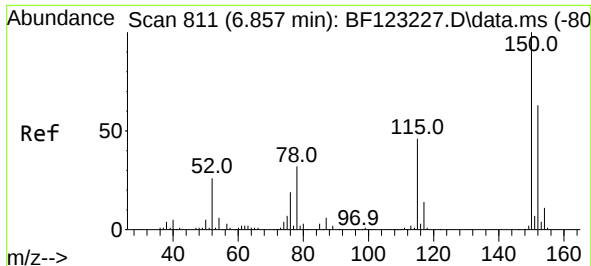

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.851 min Scan# 810
Delta R.T. -0.006 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampleId :
T-2


Tgt Ion:152 Resp: 135637
Ion Ratio Lower Upper
152 100
150 155.5 125.8 188.6
115 74.0 49.3 73.9#

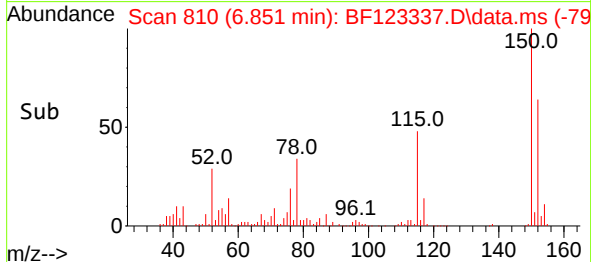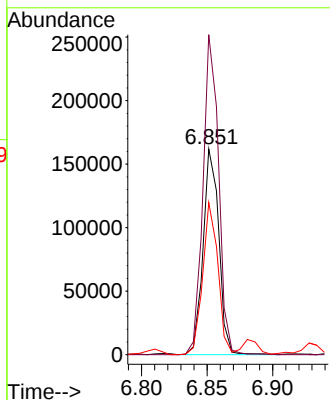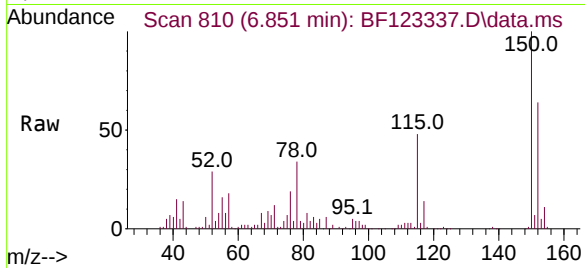

#5
2-Fluorophenol
Concen: 85.50 ng
RT: 5.475 min Scan# 576
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39

Tgt Ion:112 Resp: 805645
Ion Ratio Lower Upper
112 100
64 65.9 46.9 70.3
63 34.7 24.5 36.7


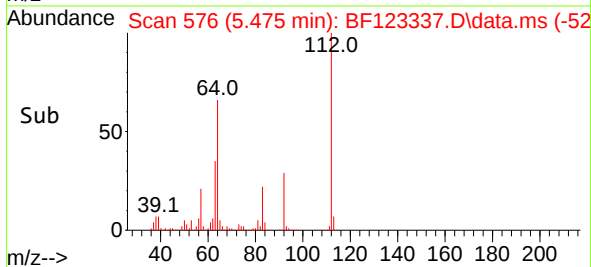
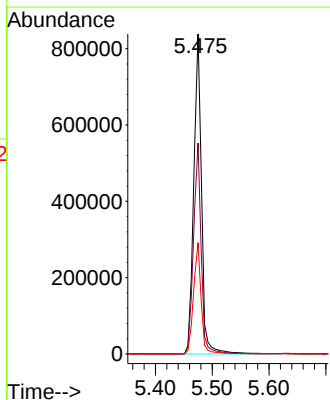
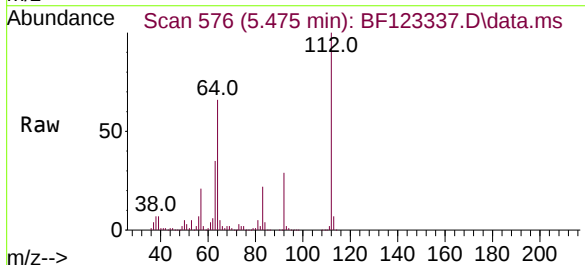


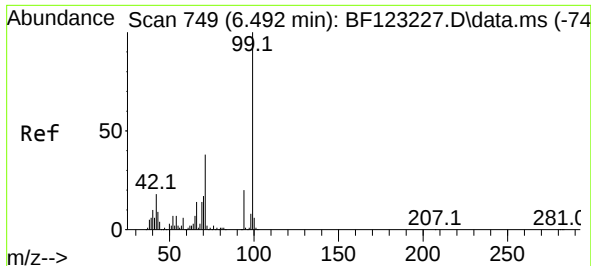

#7
Phenol-d6
Concen: 81.86 ng
RT: 6.487 min Scan# 748
Delta R.T. -0.006 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampleId :
T-2


Tgt Ion: 99 Resp: 1048011
Ion Ratio Lower Upper
99 100
42 20.6 13.8 20.6
71 40.9 26.9 40.3#

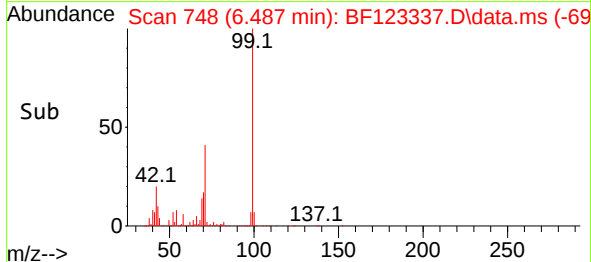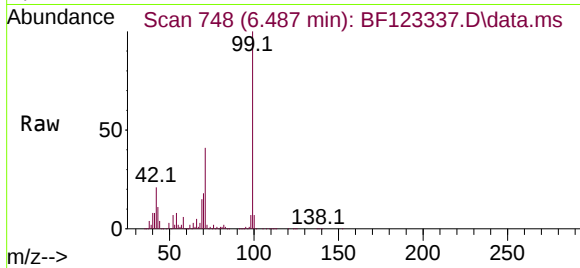

#10
Phenol
Concen: 2.14 ng
RT: 6.498 min Scan# 750
Delta R.T. -0.006 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39

Tgt Ion: 94 Resp: 29906
Ion Ratio Lower Upper
94 100
65 34.9 11.2 51.2
66 58.4 25.8 65.8


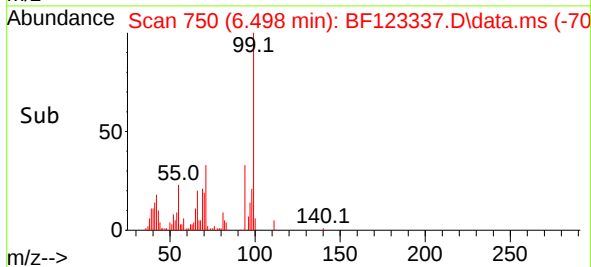

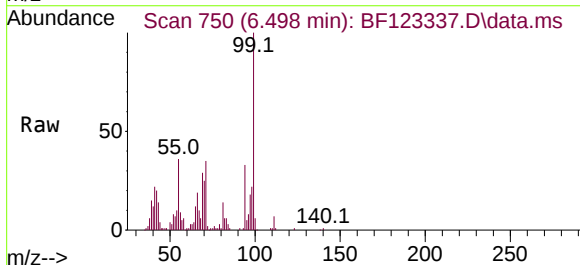


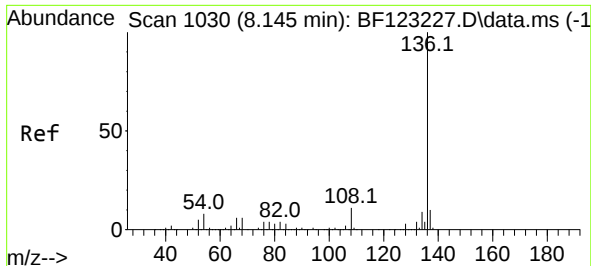

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.145 min Scan# 1030
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampled :
T-2


Tgt Ion:	136	Resp:	445475
Ion Ratio	Lower	Upper	
136	100		
137	12.2	8.8	13.2
54	10.3	5.5	8.3#
68	9.3	4.6	6.8#

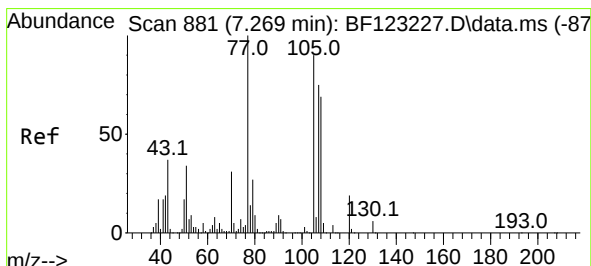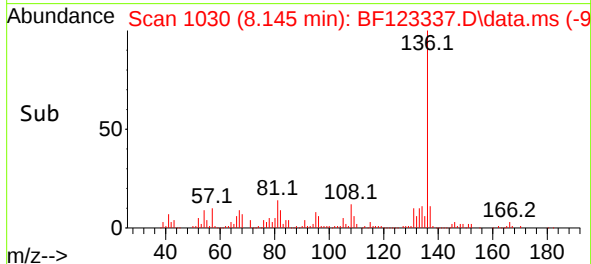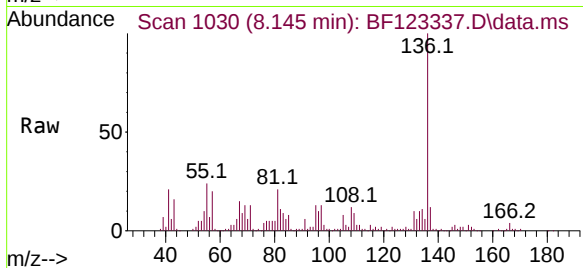

#22
Acetophenone
Concen: 30.29 ng
RT: 7.251 min Scan# 878
Delta R.T. -0.018 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39

Tgt Ion:	105	Resp:	350006
Ion Ratio	Lower	Upper	
105	100		
71	17.0	6.5	9.7#
51	4.9	24.3	36.5#
120	0.3	18.1	27.1#

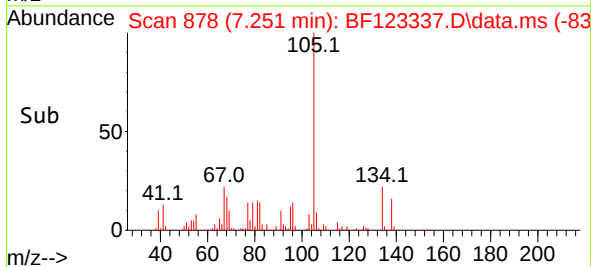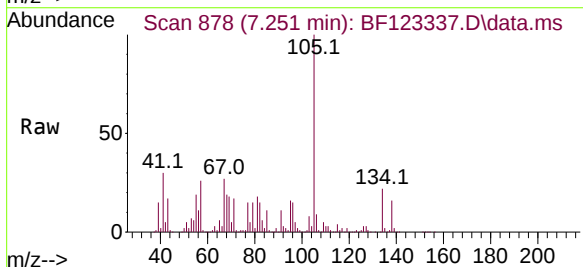

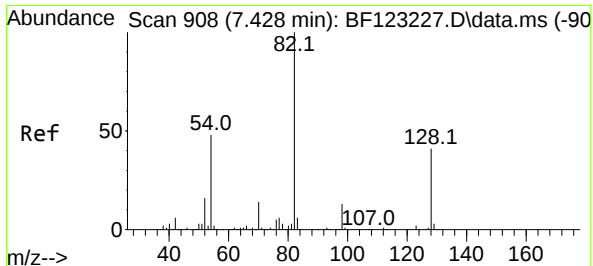

#23

Nitrobenzene-d5

Concen: 73.14 ng

RT: 7.416 min Scan# 906

Delta R.T. -0.012 min

Lab File: BF123337.D

Acq: 2 Mar 2021 15:39

Tgt Ion: 82 Resp: 711759

Ion Ratio Lower Upper

82 100

128 36.2 37.0 55.4#





54 50.9 38.4 57.6

Instrument :

BNA_F

ClientSampled :

T-2

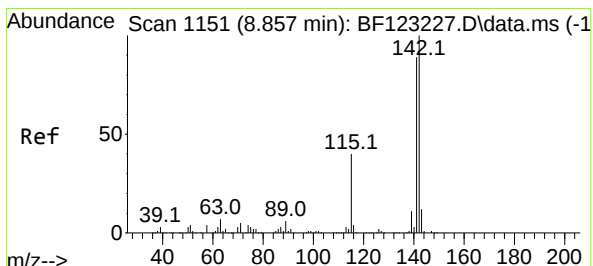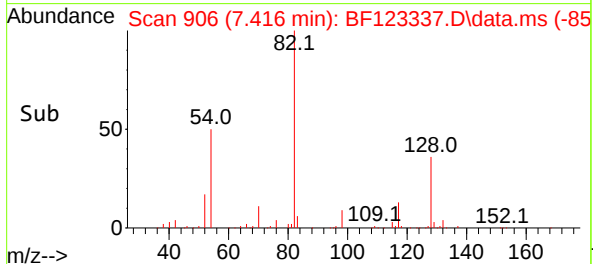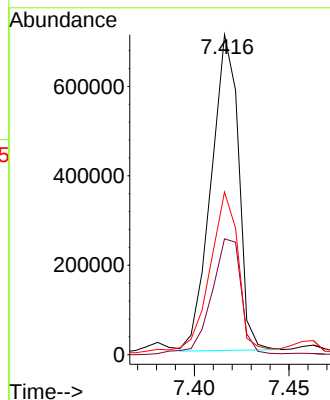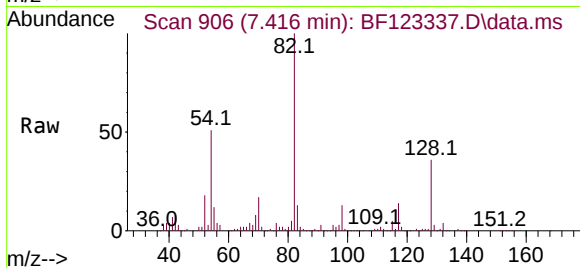

#37

2-Methylnaphthalene

Concen: 7.03 ng

RT: 8.857 min Scan# 1151

Delta R.T. 0.000 min

Lab File: BF123337.D




Acq: 2 Mar 2021 15:39


Tgt Ion:142 Resp: 114265

Ion Ratio Lower Upper

142 100

141 89.7 70.6 106.0


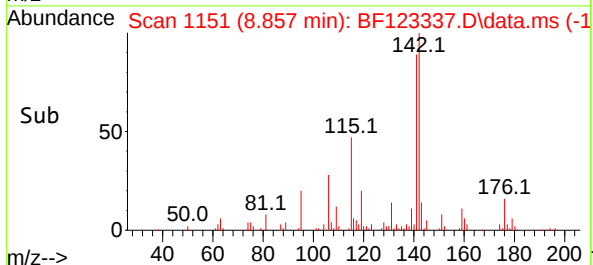
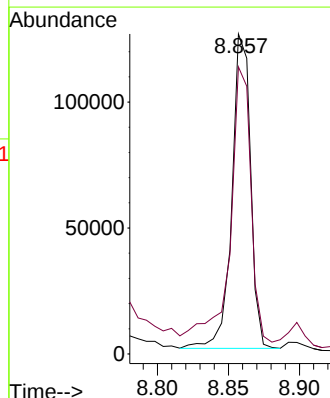
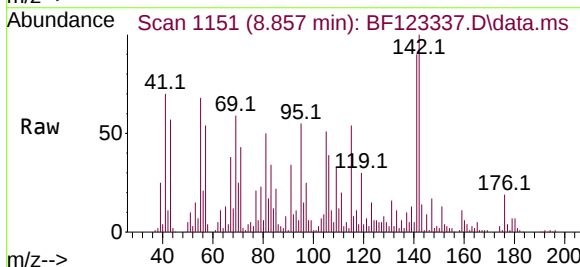




#38
1-Methylnaphthalene
Concen: 28.57 ng
RT: 8.957 min Scan# 1168
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampleId :
T-2


Tgt Ion:142 Resp: 434580
Ion Ratio Lower Upper
142 100
141 93.7 74.5 111.7

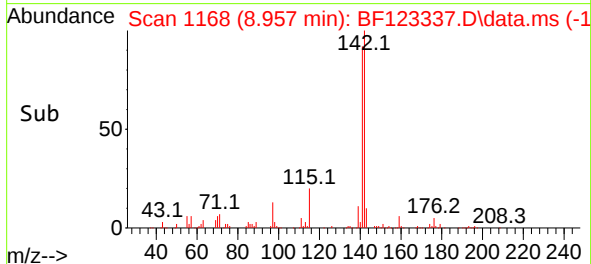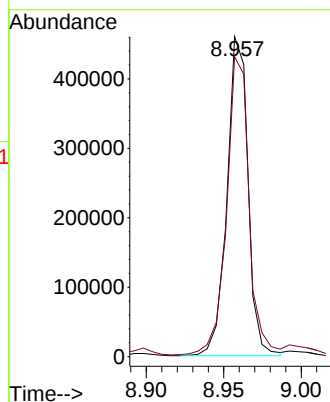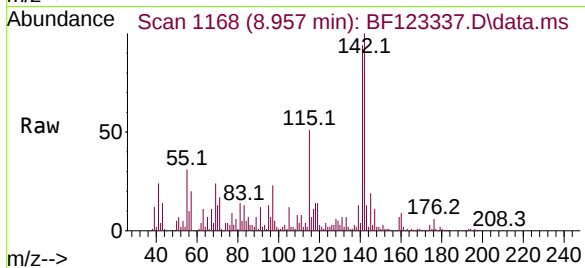

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.910 min Scan# 1330
Delta R.T. 0.006 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39

Tgt Ion:164 Resp: 277840
Ion Ratio Lower Upper
164 100
162 102.6 80.8 121.2
160 48.4 35.4 53.0



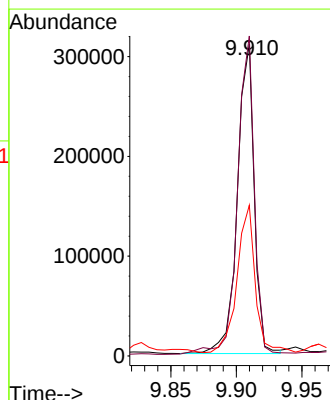
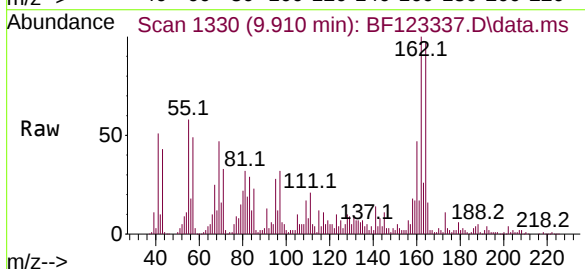


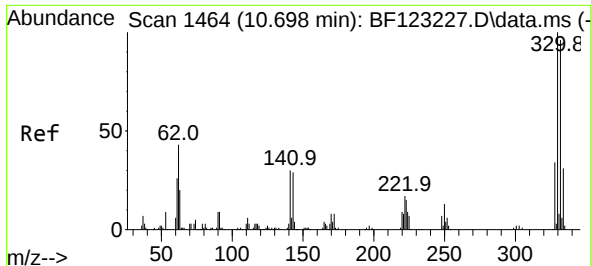

#42
2,4,6-Tribromophenol
Concen: 86.88 ng
RT: 10.704 min Scan# 1465
Delta R.T. 0.006 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampled :
T-2


Tgt Ion:330 Resp: 245803
Ion Ratio Lower Upper
330 100
332 95.7 77.5 116.3
141 41.5 23.8 35.8#

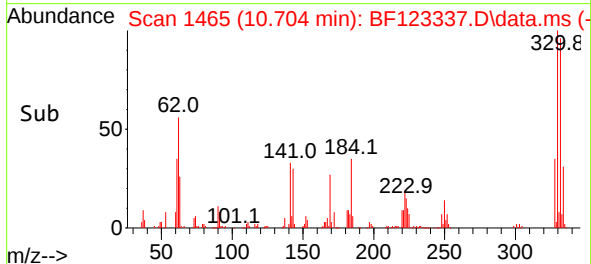

#45
2-Fluorobiphenyl
Concen: 55.66 ng
RT: 9.222 min Scan# 1213
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39

Tgt Ion:172 Resp: 1076555
Ion Ratio Lower Upper
172 100
171 37.0 29.6 44.4
170 24.1 19.5 29.3


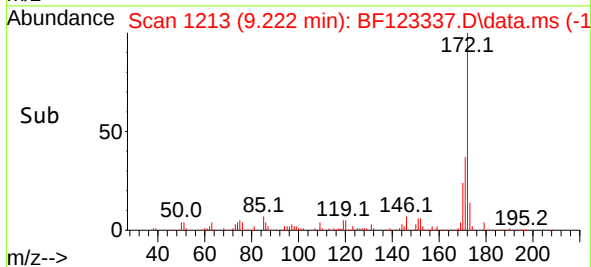

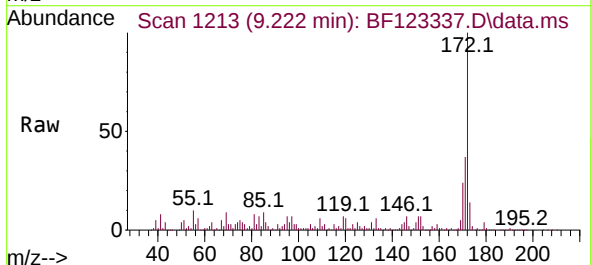


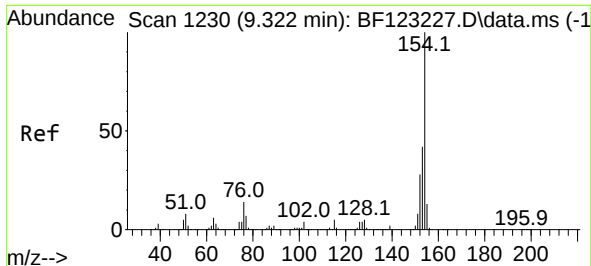

#46
1,1'-Biphenyl
Concen: 3.97 ng
RT: 9.322 min Scan# 1230
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampled :
T-2


Tgt Ion:154 Resp: 91610
Ion Ratio Lower Upper
154 100
153 37.6 21.8 61.8
76 11.5 0.0 33.4

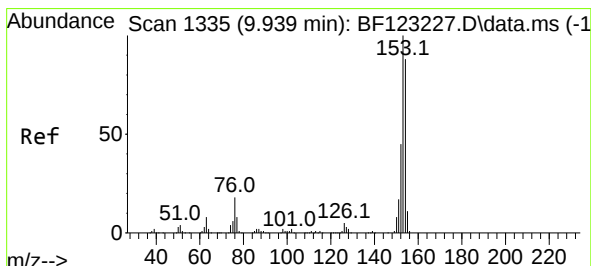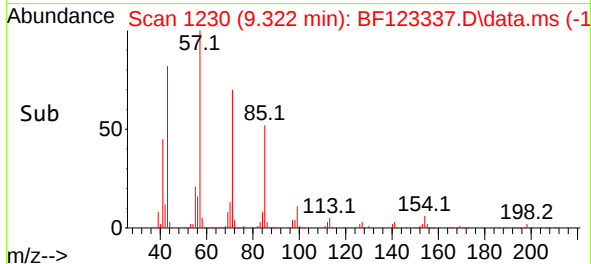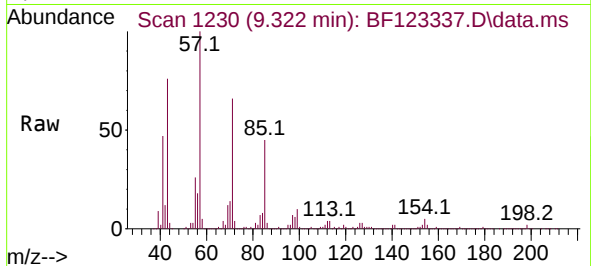

#52
Acenaphthene
Concen: 4.51 ng
RT: 9.939 min Scan# 1335
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39

Tgt Ion:154 Resp: 85847
Ion Ratio Lower Upper
154 100
153 124.4 89.0 133.6
152 73.4 42.7 64.1#


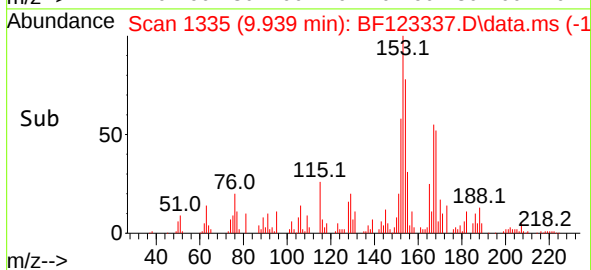

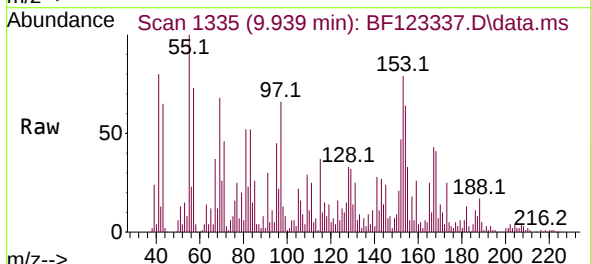


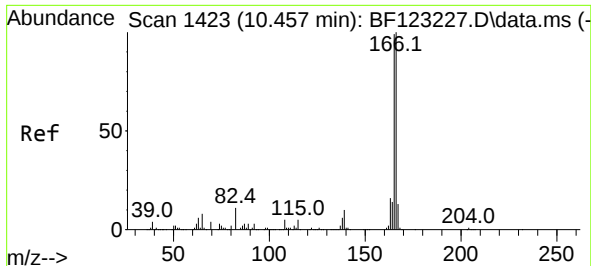

#58
Fluorene
Concen: 8.72 ng
RT: 10.457 min Scan# 1423
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampleId :
T-2


Tgt Ion:166 Resp: 176759
Ion Ratio Lower Upper
166 100
165 106.0 79.4 119.0
167 25.2 10.9 16.3#

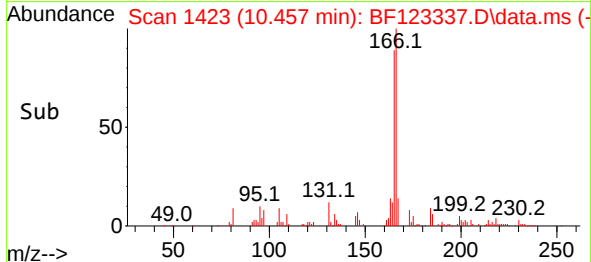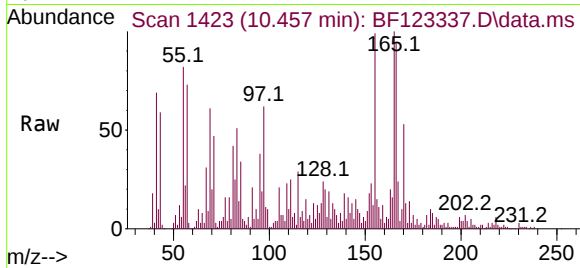

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.398 min Scan# 1583
Delta R.T. 0.006 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39

Tgt Ion:188 Resp: 488550
Ion Ratio Lower Upper
188 100
94 11.9 7.4 11.2#
80 13.1 8.2 12.4#


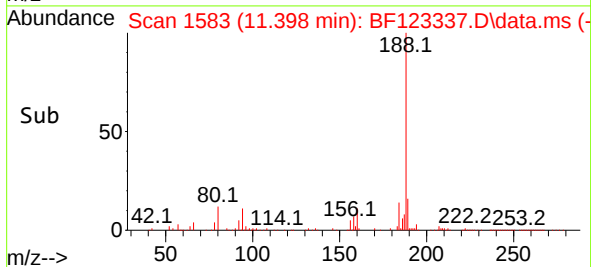

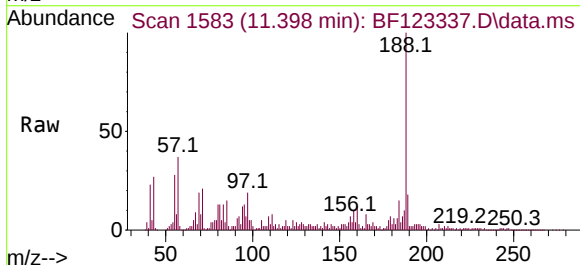




#71
Phenanthrene
Concen: 19.22 ng
RT: 11.427 min Scan# 1588
Delta R.T. 0.006 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampled :
T-2


Tgt Ion:178 Resp: 555151
Ion Ratio Lower Upper
178 100
176 19.6 16.2 24.2
179 18.8 12.7 19.1

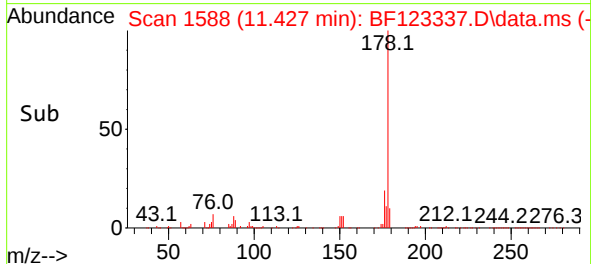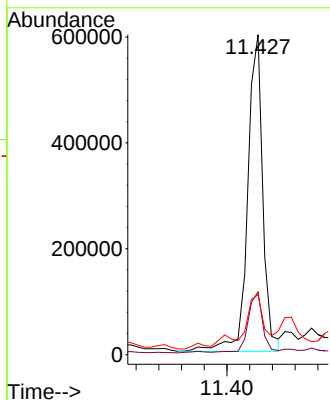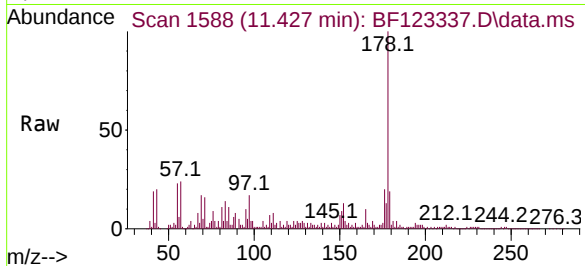

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.039 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39

Tgt Ion:240 Resp: 344619
Ion Ratio Lower Upper
240 100
120 11.6 8.6 12.8
236 25.5 20.3 30.5


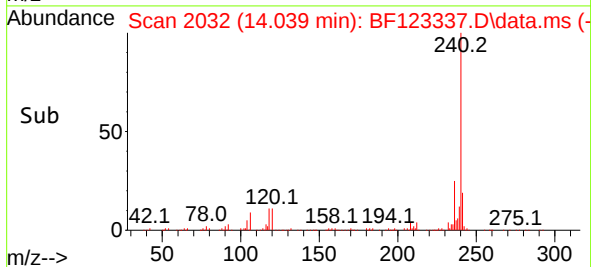
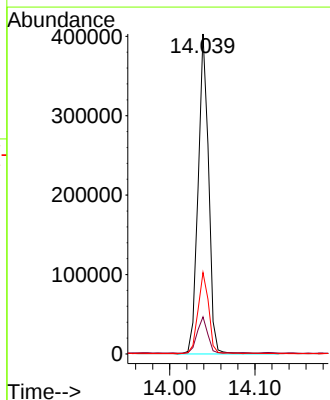
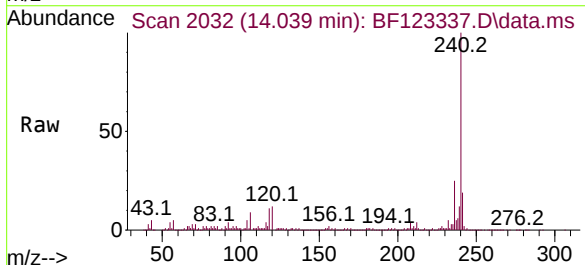




#78
Pyrene
Concen: 4.77 ng
RT: 12.845 min Scan# 1829
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39




Instrument :
BNA_F
ClientSampled :
T-2


Tgt Ion:	202	Resp:	128418
Ion Ratio	Lower	Upper	
202	100		
200	21.5	17.6	26.4
203	22.6	14.6	21.8#

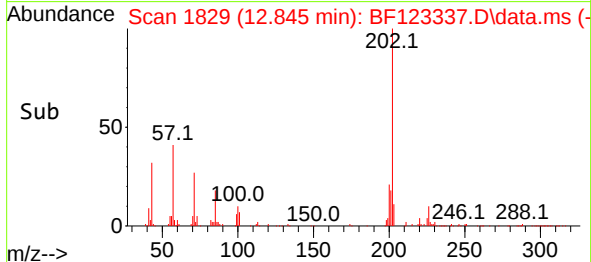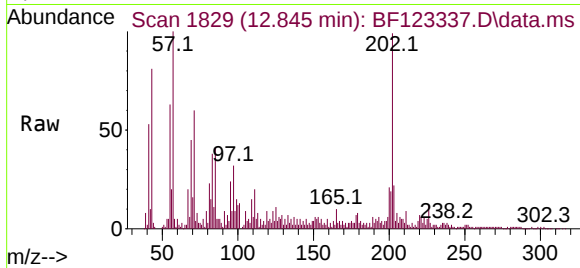

#79
Terphenyl-d14
Concen: 60.90 ng
RT: 12.986 min Scan# 1853
Delta R.T. 0.000 min
Lab File: BF123337.D
Acq: 2 Mar 2021 15:39


Tgt Ion:	244	Resp:	1091510
Ion Ratio	Lower	Upper	
244	100		
212	7.5	5.7	8.5
122	12.1	8.3	12.5

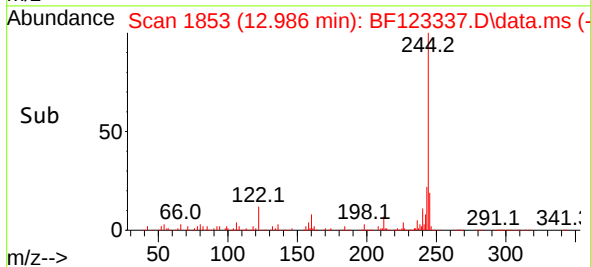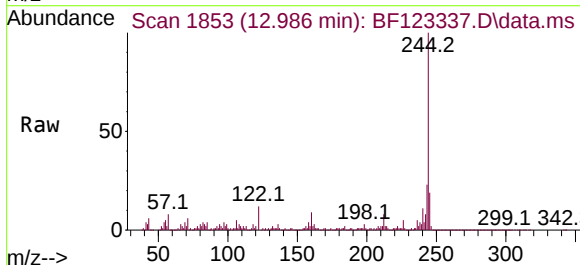



#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.515 min Scan# 2283
 Delta R.T. 0.000 min
 Lab File: BF123337.D
 Acq: 2 Mar 2021 15:39

Instrument :
 BNA_F
 ClientSampleId :
 T-2

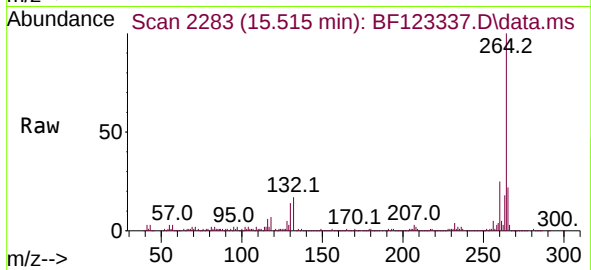

Tgt Ion:264 Resp: 300130
 Ion Ratio Lower Upper
 264 100
 260 24.9 18.6 28.0
 265 22.0 17.0 25.6

