


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030221\
 Data File : BF123331.D
 Acq On : 2 Mar 2021 11:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

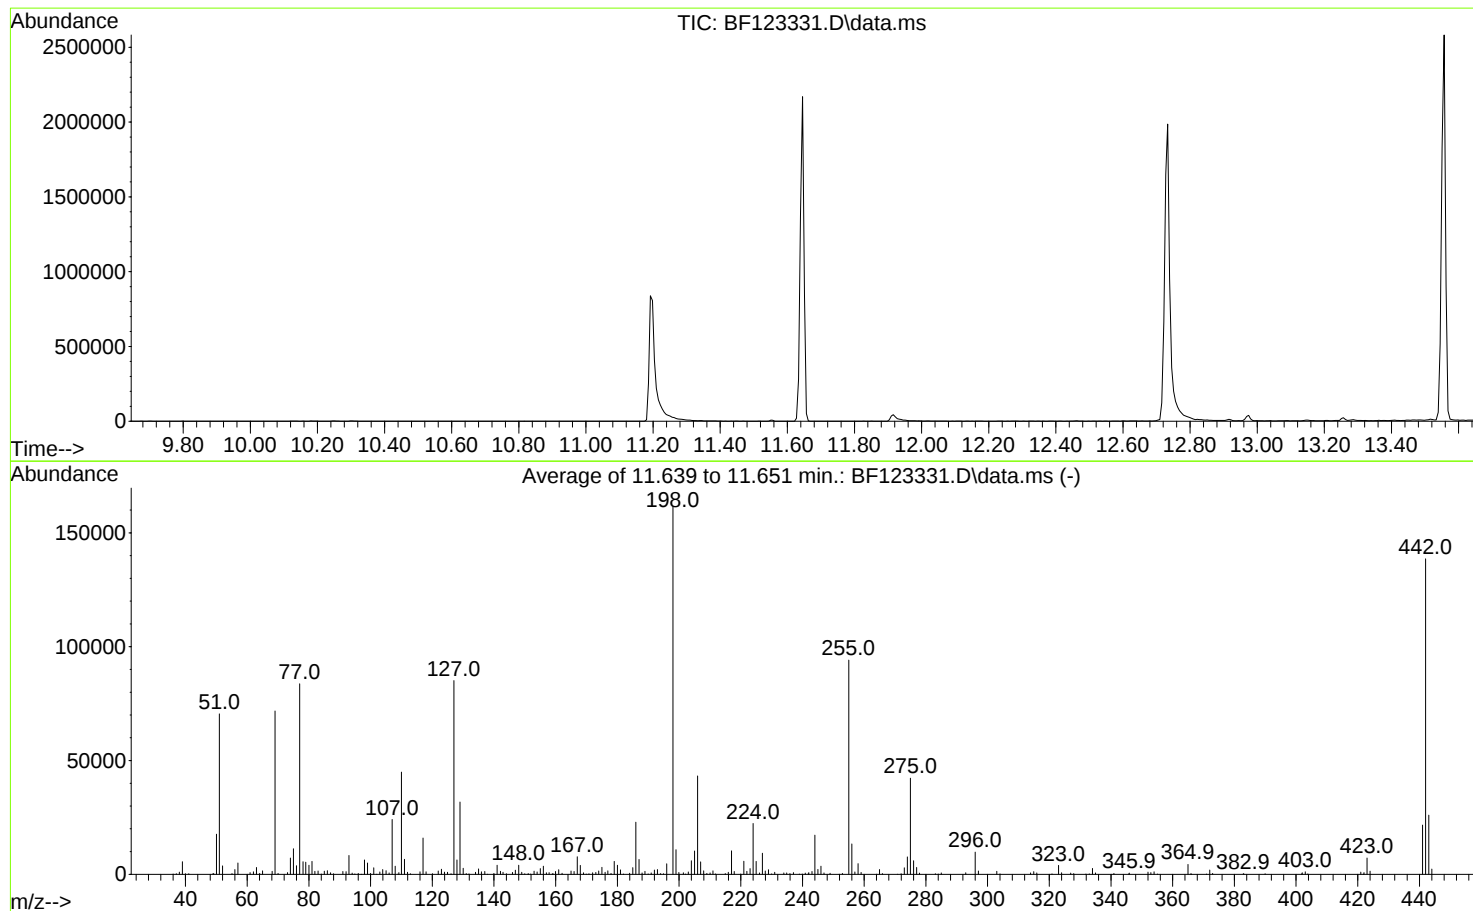

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	70464	PASS
68	69	0.00	2	1.9	1358	PASS
69	198	0.00	100	44.4	71773	PASS
70	69	0.00	2	0.6	431	PASS
127	198	10	80	52.7	85131	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	161568	PASS
199	198	5	9	6.7	10816	PASS
275	198	10	60	26.1	42243	PASS
365	198	1	100	2.7	4363	PASS
441	198	0.01	100	13.4	21627	PASS
442	442	50	100	100.0	138589	PASS
443	442	15	24	18.8	26008	PASS

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/2/2021	BNA_F	<u>BF123331.D</u>
Compound Name	Response	Retention Time
DDT	380438	13.55
DDD	4350	13.25
DDE	1725	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6075	386513	1.57

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030221\
Data File : BF123331.D
Acq On : 2 Mar 2021 11:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 02 12:28:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

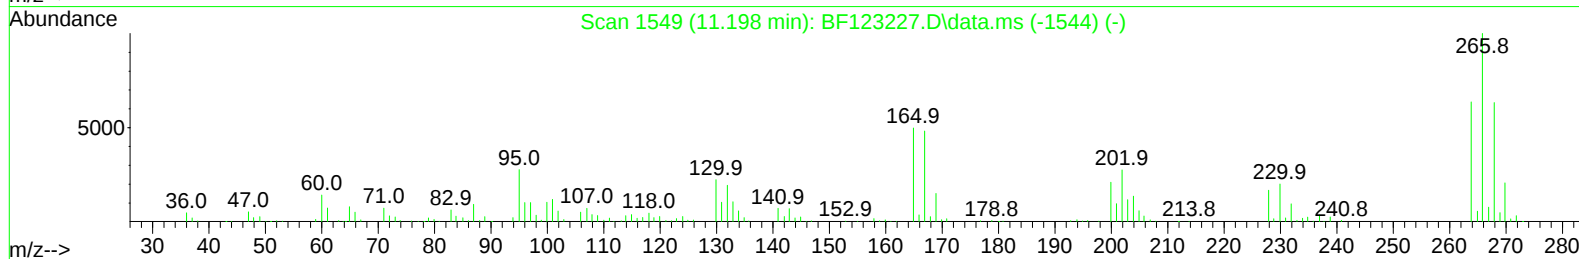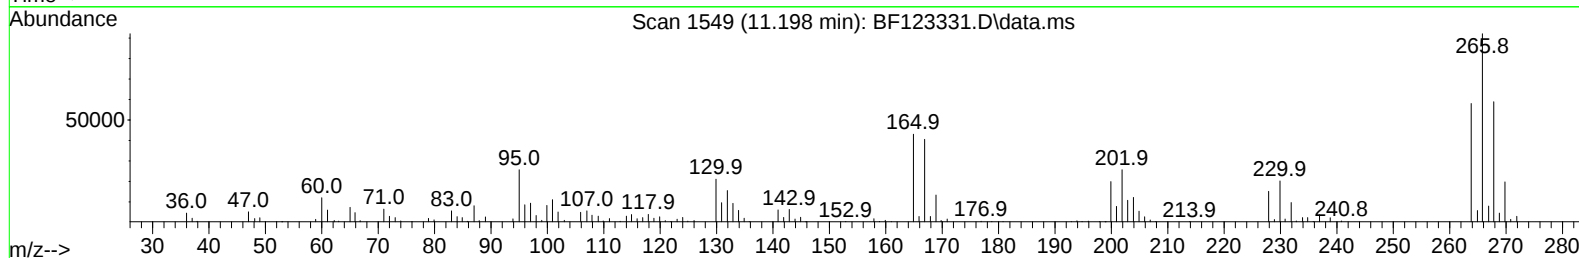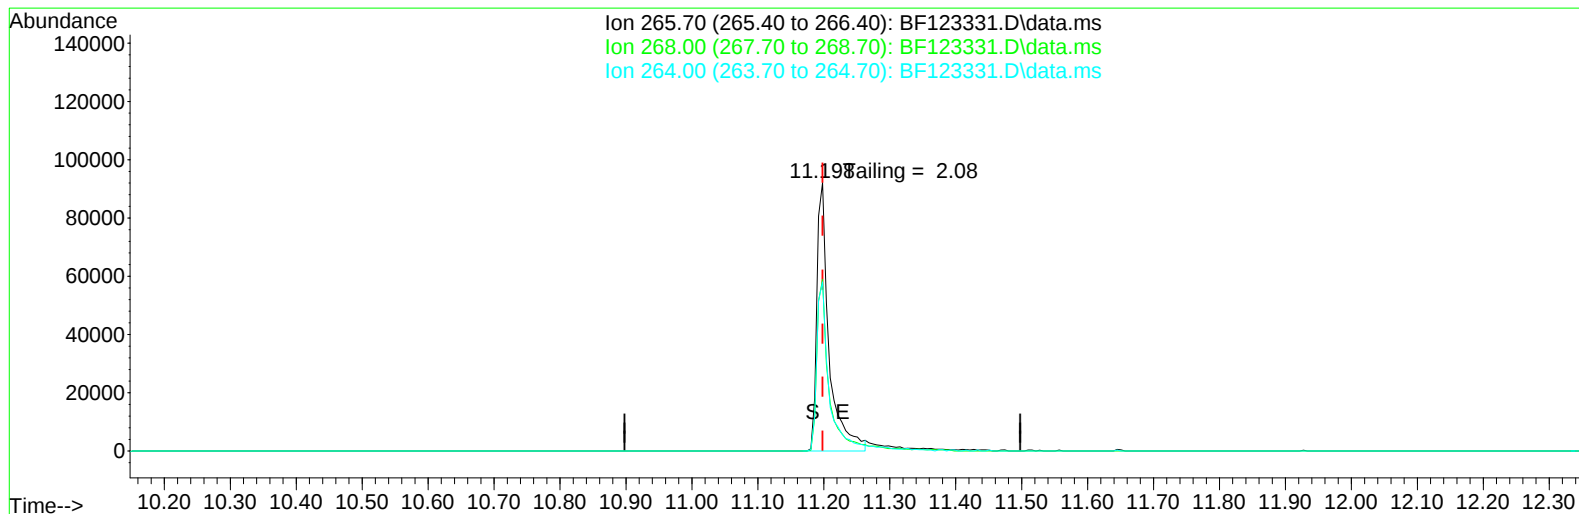

TIC: BF123331.D\data.ms

(70) Pentachlorophenol (C)

11.198min (0.000) 26468.49 ng




response 126485

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.93
264.00	62.30	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030221\
Data File : BF123331.D
Acq On : 2 Mar 2021 11:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 02 12:28:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

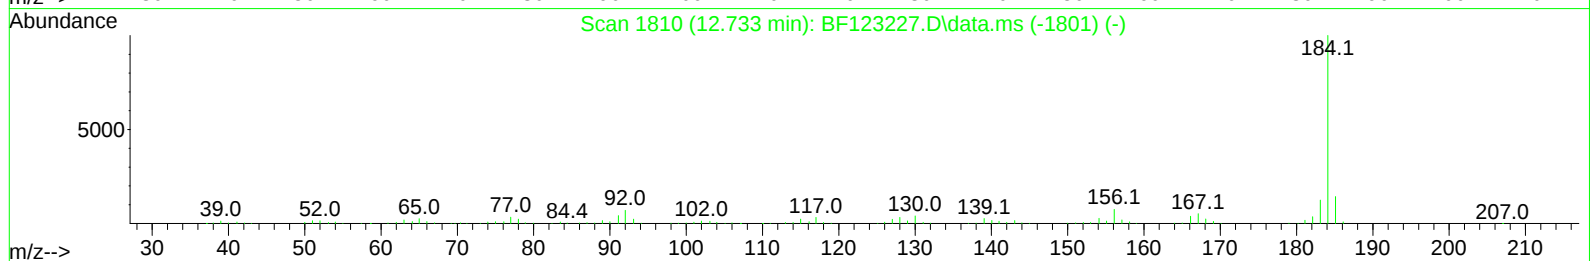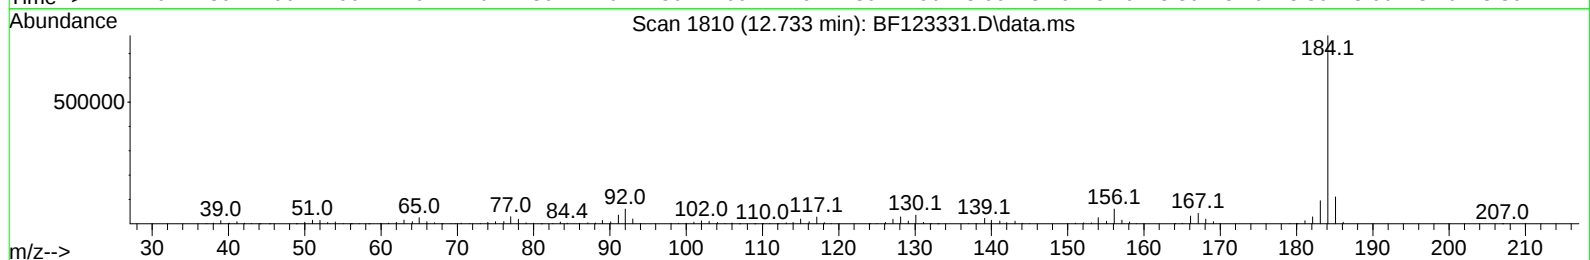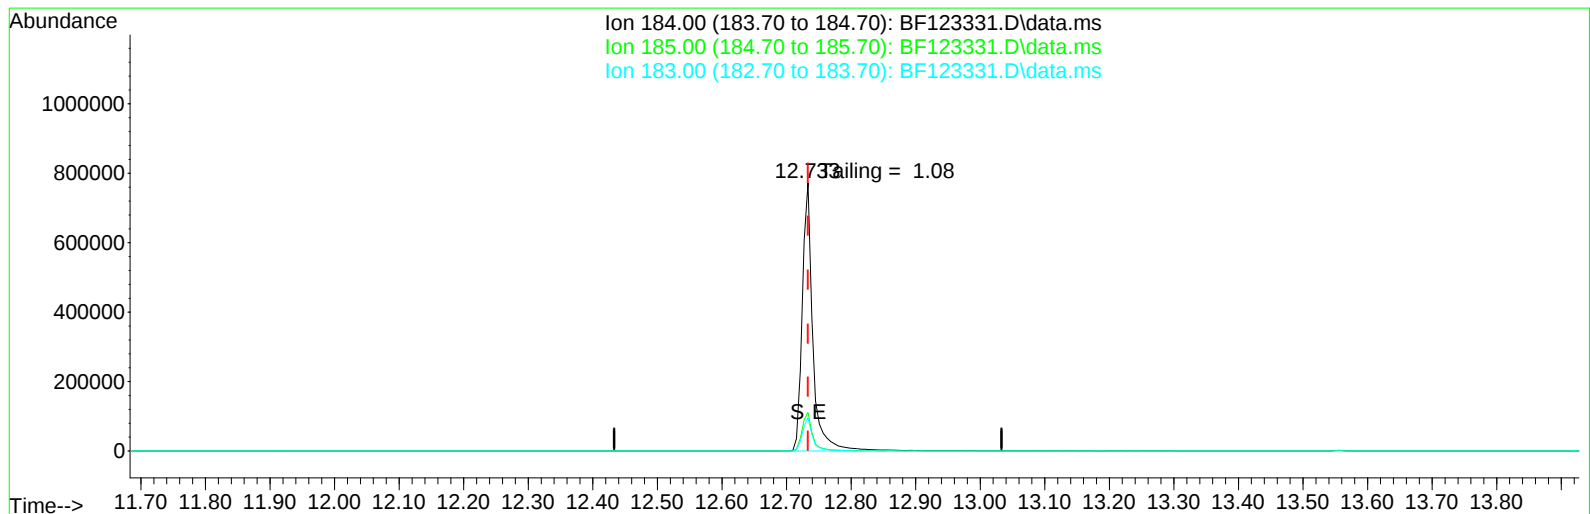

TIC: BF123331.D\data.ms

(77) Benzidine

12.733min (0.000) 0.00 ng

response 883362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.33
183.00	12.10	12.32
0.00	0.00	0.00