
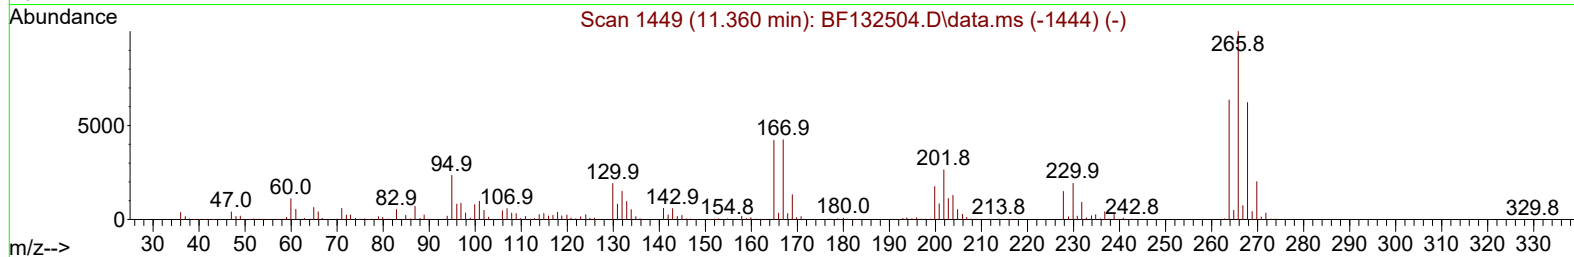
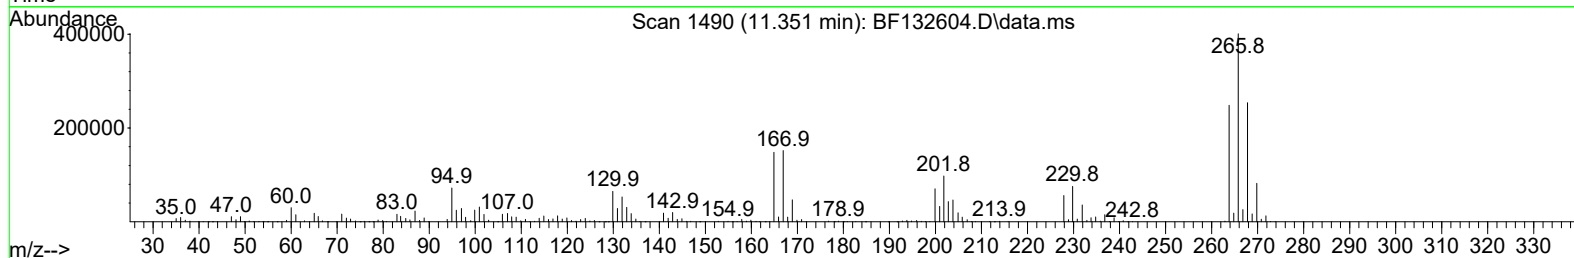


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
Data File : BF132604.D
Acq On : 02 Mar 2023 12:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 05:45:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

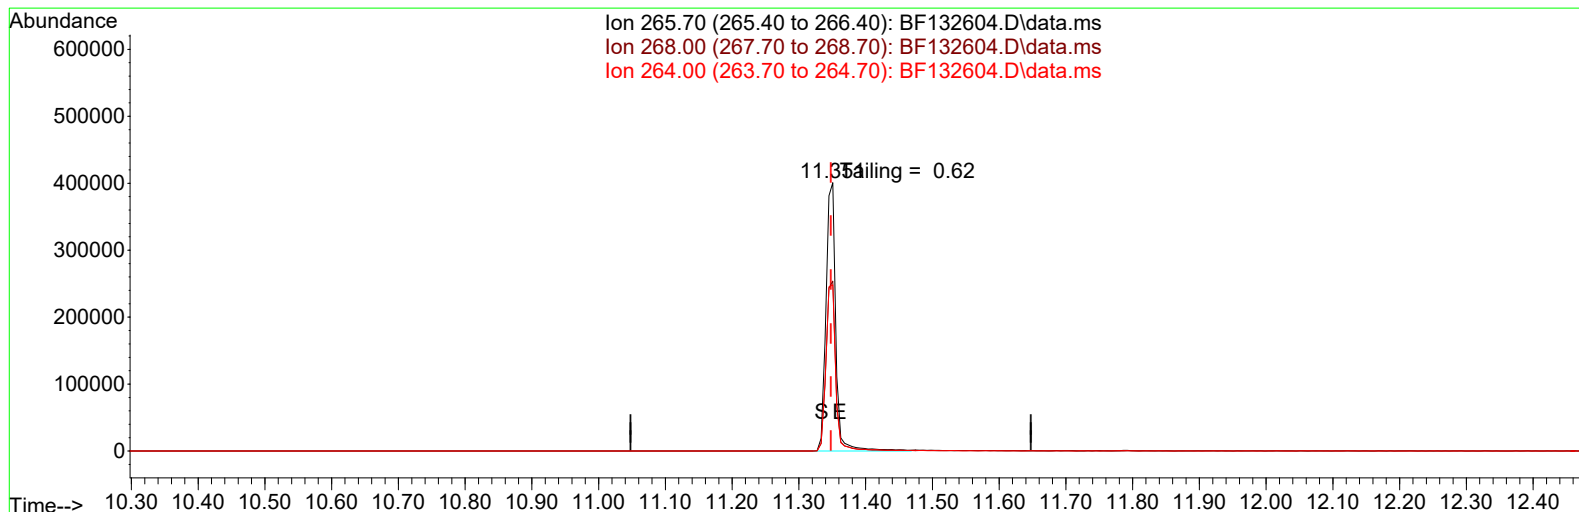

TIC: BF132604.D\data.ms

(70) Pentachlorophenol (C)




11.351min (+ 0.003) 217831.32 ng

response 408782

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.31
264.00	63.60	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
Data File : BF132604.D
Acq On : 02 Mar 2023 12:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 05:45:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

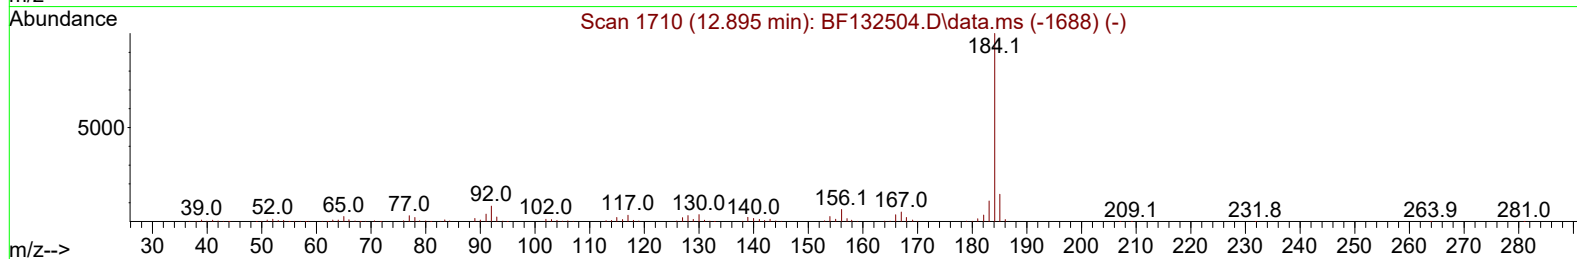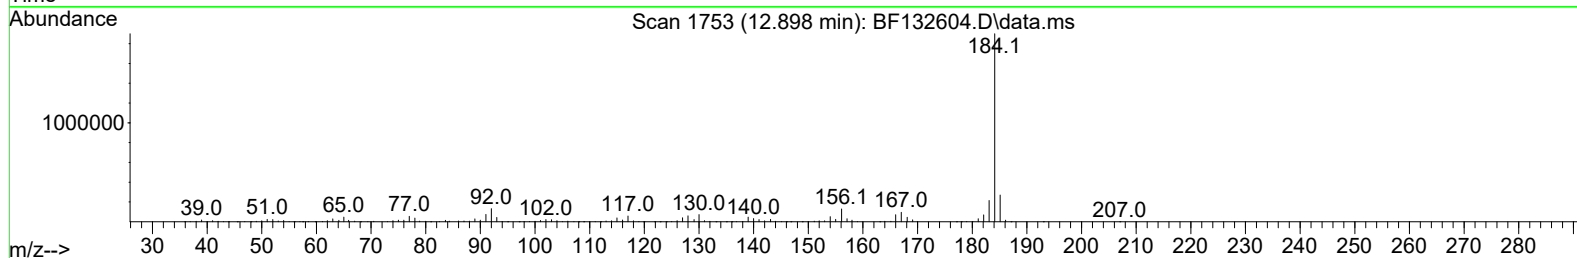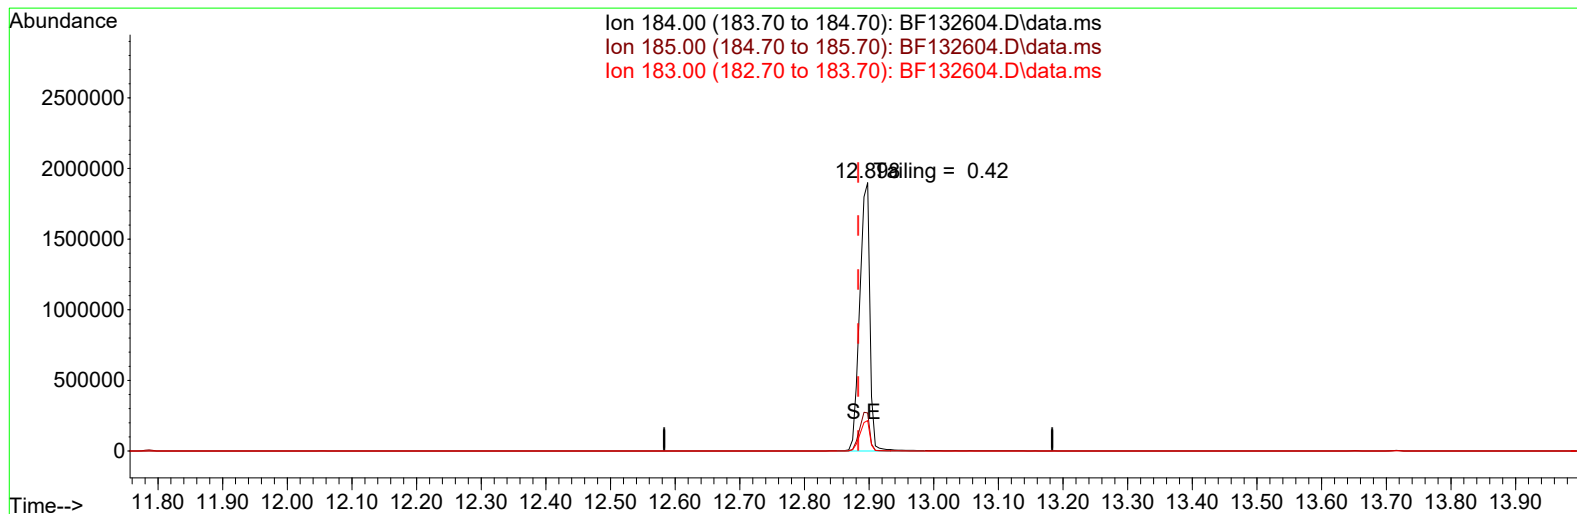

TIC: BF132604.D\data.ms

(77) Benzidine

12.898min (+ 0.015) 77579.45 ng

response 2092464

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.22
183.00	10.90	11.36
0.00	0.00	0.00