

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
 Data File : BF132620.D
 Acq On : 02 Mar 2023 21:54
 Operator : CG\JU
 Sample : 01742-01 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RBR251669

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.122	257	261	268	rVB2	23766	30124	2.08%	0.264%
2	5.216	443	447	458	rVB	278588	290499	20.05%	2.545%
3	5.616	512	515	524	rVB	778434	692171	47.78%	6.063%
4	6.616	682	685	705	rVB	840605	696000	48.04%	6.096%
5	6.998	747	750	754	rBV	1483211	1199183	82.78%	10.504%
6	7.557	842	845	849	rBV	541982	414700	28.63%	3.632%
7	8.287	965	969	972	rBV	1830974	1448680	100.00%	12.689%
8	9.357	1148	1151	1155	rBV	1036150	765769	52.86%	6.708%
9	9.428	1160	1163	1167	rBV	20526	18942	1.31%	0.166%
10	9.751	1215	1218	1222	rBV3	24035	23222	1.60%	0.203%
11	9.957	1250	1253	1257	rVB2	26698	26188	1.81%	0.229%
12	10.045	1265	1268	1272	rVB	1557911	1347979	93.05%	11.807%
13	10.463	1334	1339	1341	rBV3	23804	29701	2.05%	0.260%
14	10.757	1387	1389	1394	rVB	19513	18072	1.25%	0.158%
15	10.839	1399	1403	1411	rVV	381116	346579	23.92%	3.036%
16	10.951	1417	1422	1425	rBV	48585	55754	3.85%	0.488%
17	11.422	1498	1502	1504	rBV	25689	25446	1.76%	0.223%
18	11.545	1519	1523	1526	rBV	1460910	1242775	85.79%	10.886%
19	11.769	1559	1561	1566	rBV5	16637	22274	1.54%	0.195%
20	11.816	1567	1569	1572	rVB3	22732	18924	1.31%	0.166%
21	12.057	1607	1610	1616	rBV7	24101	45986	3.17%	0.403%
22	12.228	1637	1639	1643	rBV4	16115	18384	1.27%	0.161%
23	12.622	1704	1706	1711	rVB4	18111	19065	1.32%	0.167%
24	12.763	1728	1730	1733	rBV	38676	39188	2.71%	0.343%
25	12.998	1767	1770	1777	rVB2	66873	75413	5.21%	0.661%
26	13.133	1789	1793	1796	rBV	749977	607805	41.96%	5.324%
27	13.322	1823	1825	1827	rBV3	29167	23842	1.65%	0.209%
28	14.204	1971	1975	1979	rBV	1165935	1044125	72.07%	9.146%
29	15.763	2235	2240	2246	rVB	619476	829661	57.27%	7.267%




Sum of corrected areas: 11416451

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
Data File : BF132620.D
Acq On : 02 Mar 2023 21:54
Operator : CG\JU
Sample : 01742-01 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RBR251669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

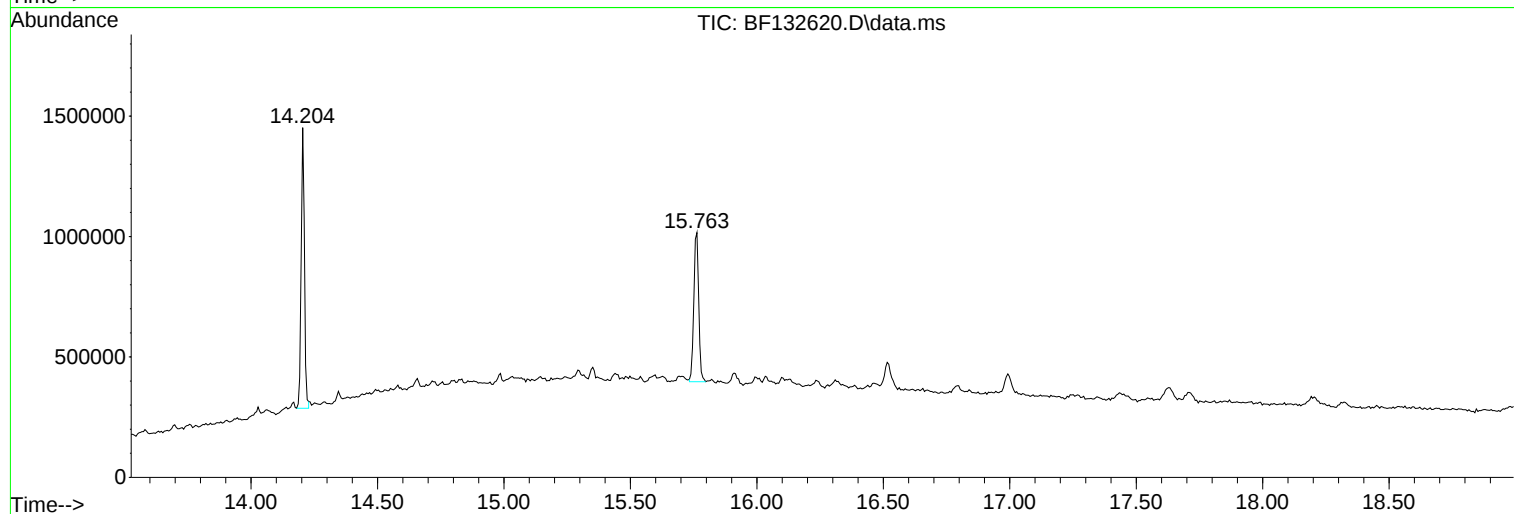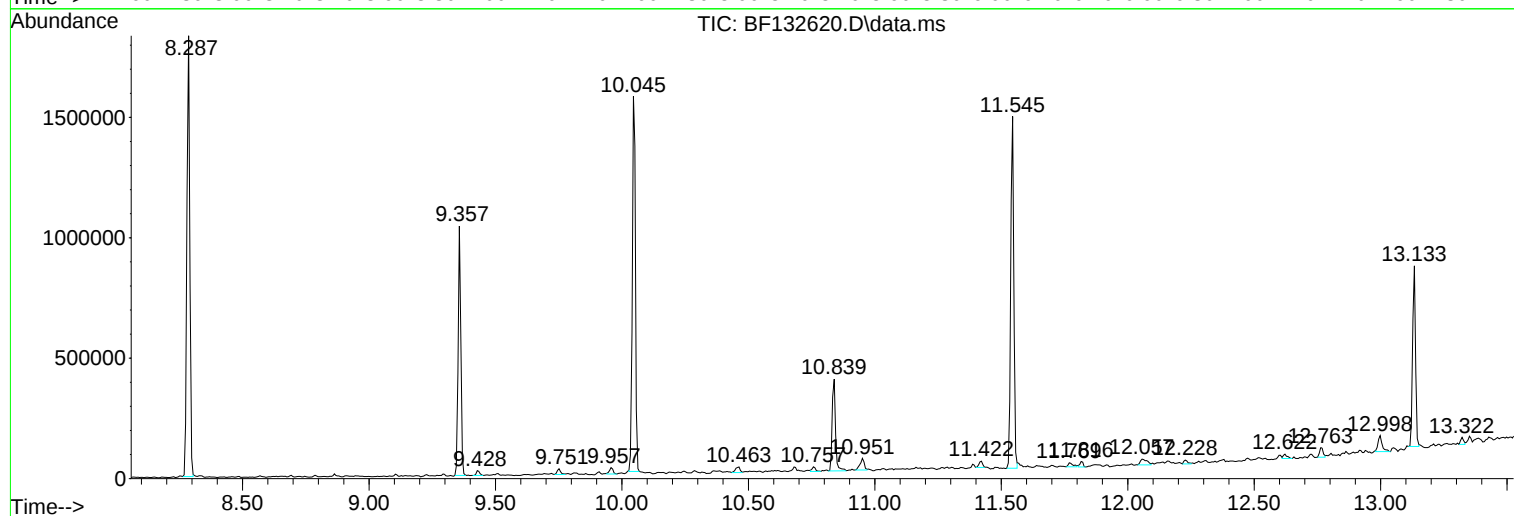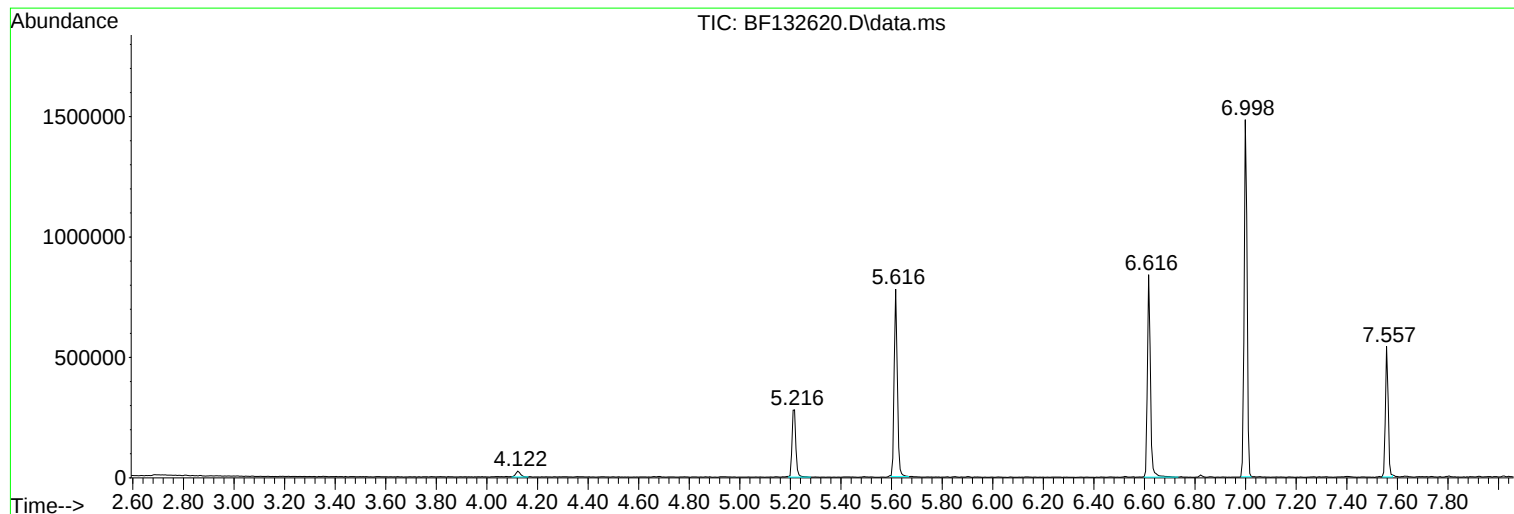

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
Data File : BF132620.D
Acq On : 02 Mar 2023 21:54
Operator : CG\JU
Sample : 01742-01 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RBR251669










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.216	4.84 ng	290499	1,4-Dichlorobenzene-d4	6.998

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

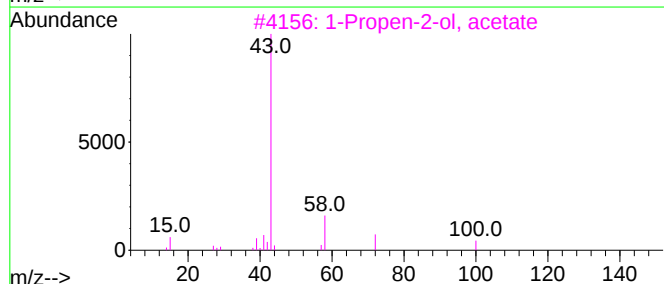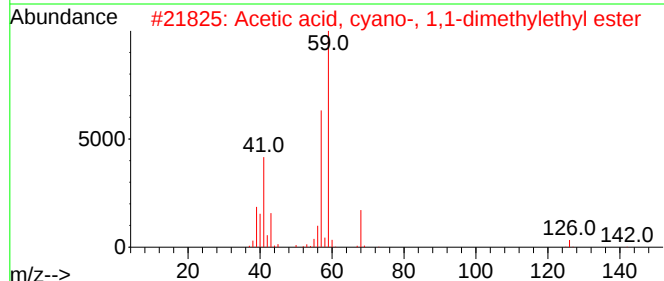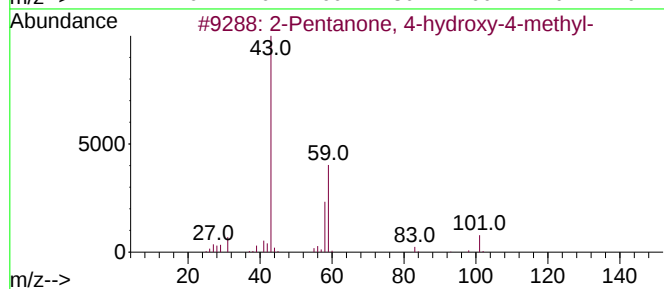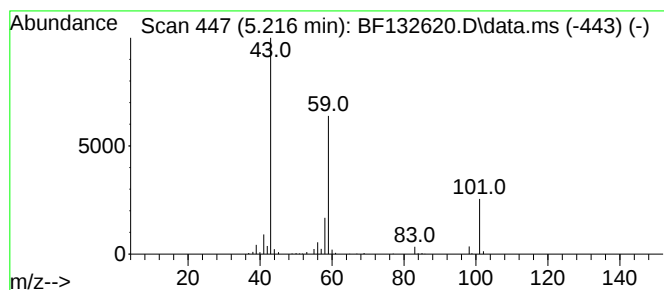

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
Data File : BF132620.D
Acq On : 02 Mar 2023 21:54
Operator : CG\JU
Sample : 01742-01 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RBR251669

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.216	4.8	ng	290499	1	6.998	1199180	20.0