


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
Data File : BF132604.D
Acq On : 02 Mar 2023 12:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 24 23:17:30 2023

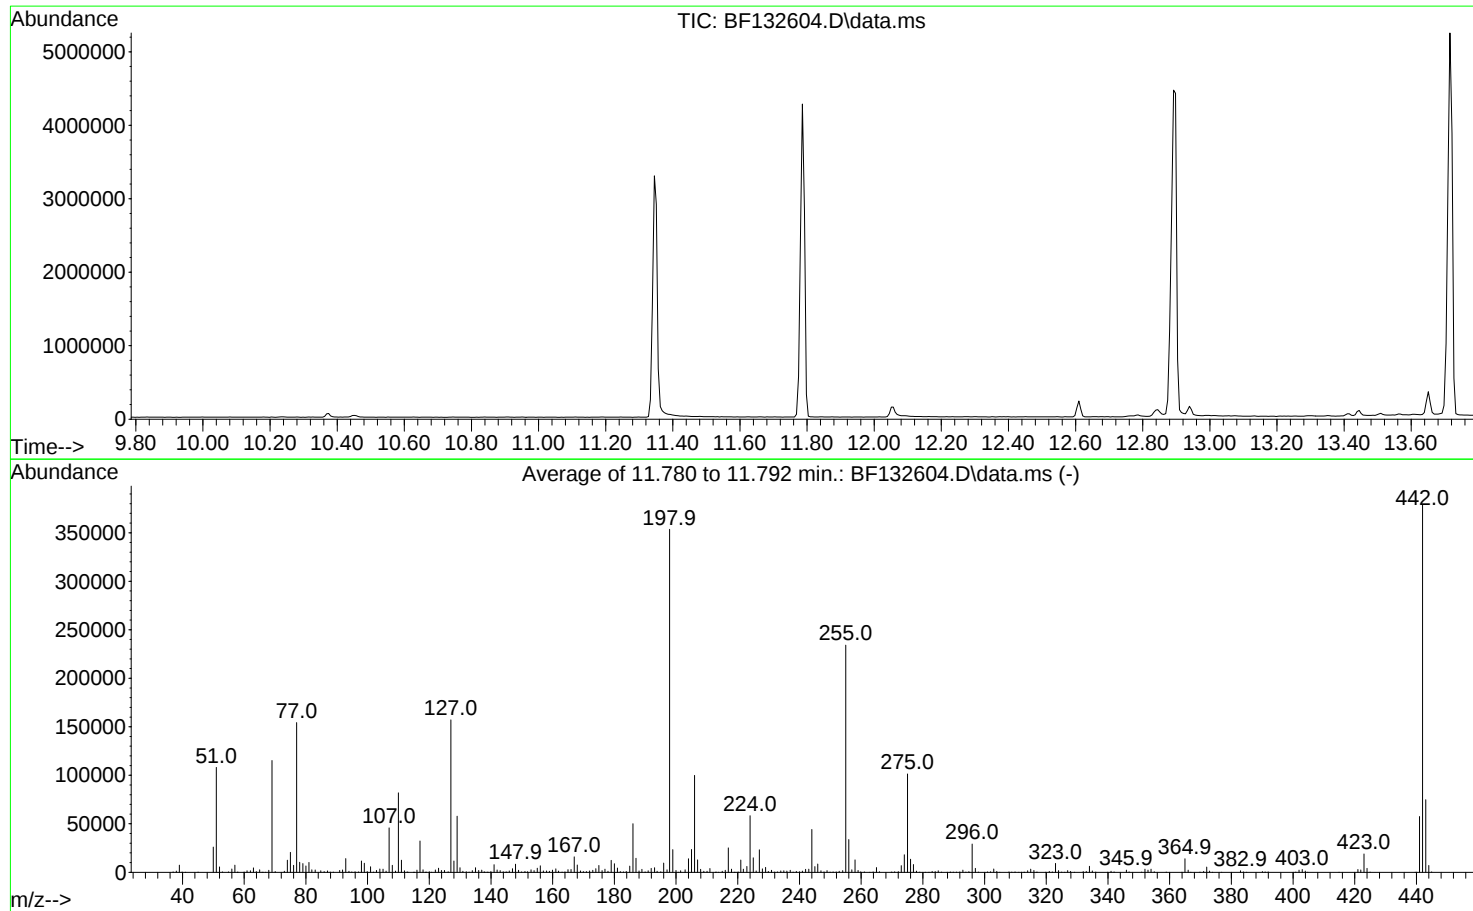




AutoFind: Scans 1563, 1564, 1565; Background Corrected with Scan 1558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	108192	PASS
68	69	0.00	2	1.9	2136	PASS
69	198	0.00	100	32.6	115160	PASS
70	69	0.00	2	0.6	732	PASS
127	198	10	80	44.5	157157	PASS
197	198	0.00	2	0.7	2620	PASS
198	198	100	100	100.0	353515	PASS
199	198	5	9	6.6	23429	PASS
275	198	10	60	28.7	101371	PASS
365	198	1	100	3.9	13897	PASS
441	198	0.01	100	16.3	57459	PASS
442	442	50	100	100.0	379221	PASS
443	442	15	24	19.7	74880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
Data File : BF132604.D
Acq On : 02 Mar 2023 12:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 03 05:45:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

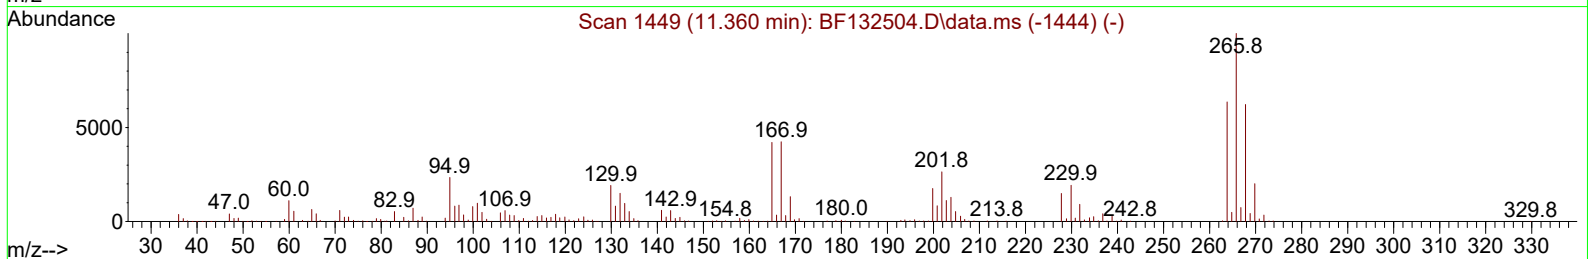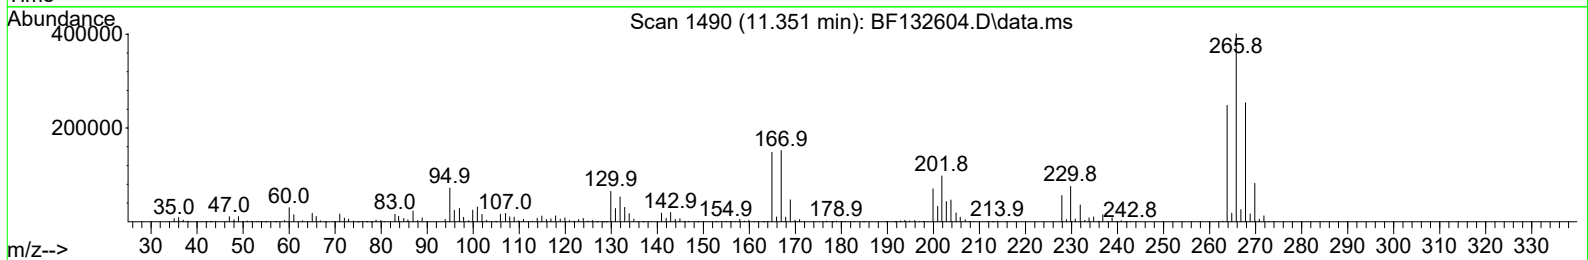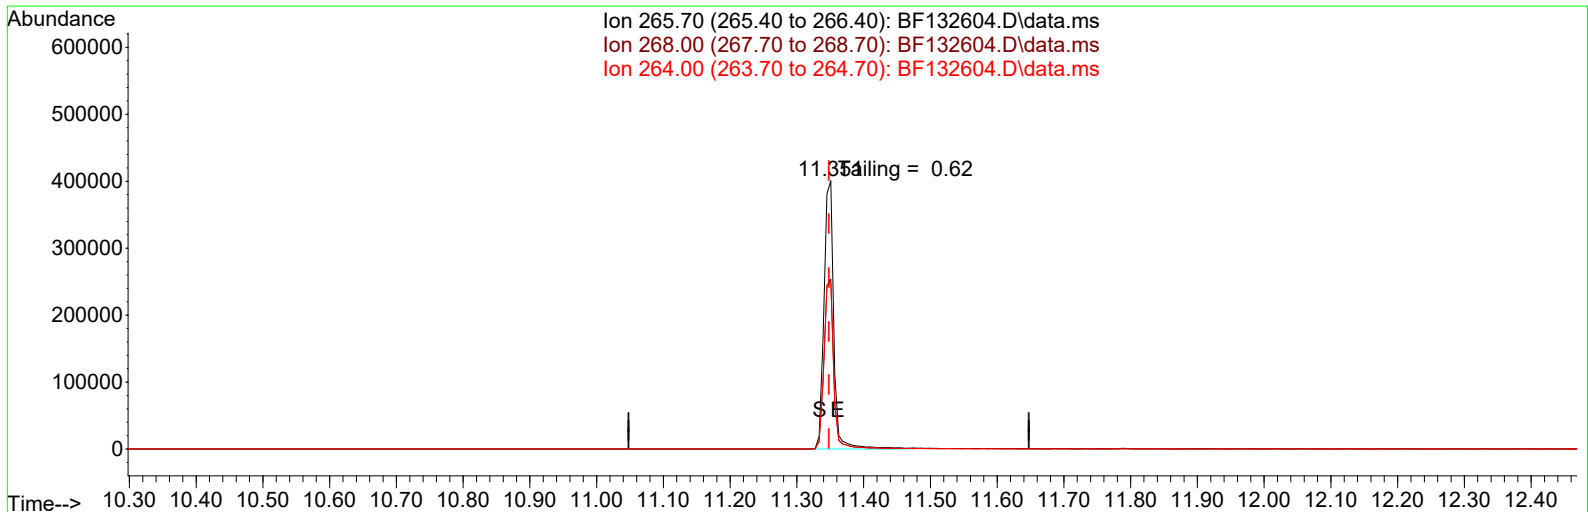

TIC: BF132604.D\data.ms

(70) Pentachlorophenol (C)

11.351min (+ 0.003) 217831.32 ng




response 408782

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.31
264.00	63.60	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030223\
Data File : BF132604.D
Acq On : 02 Mar 2023 12:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 03 05:45:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

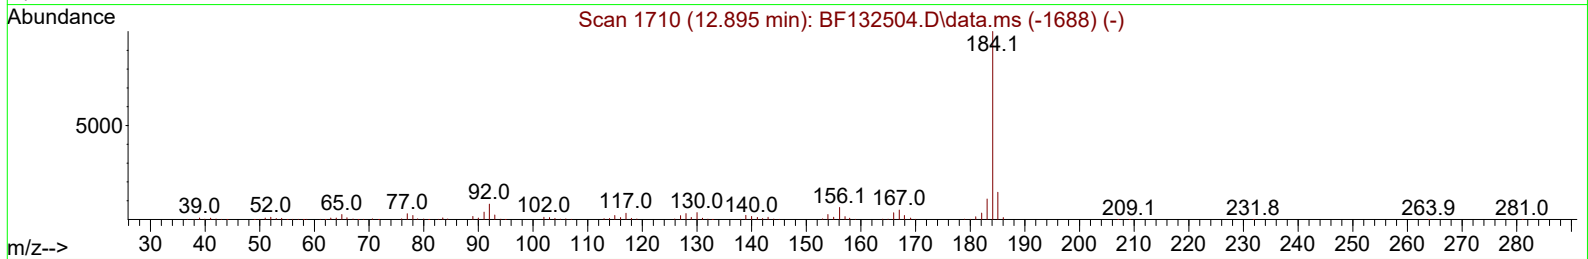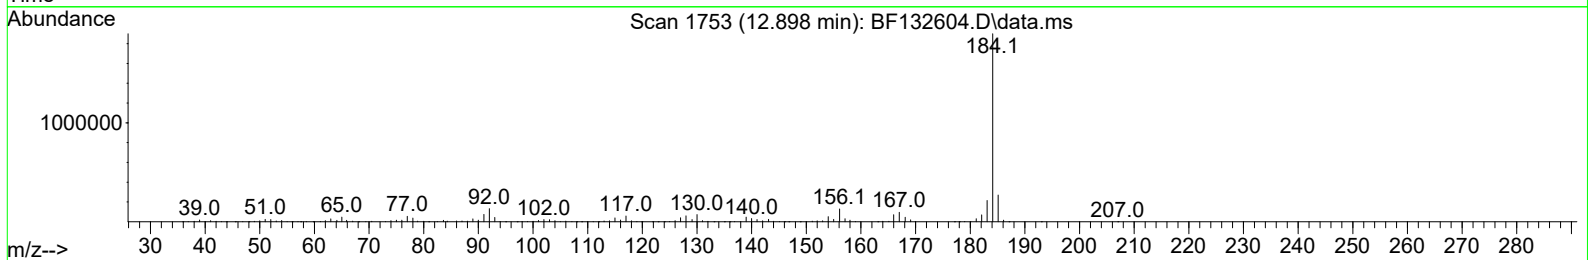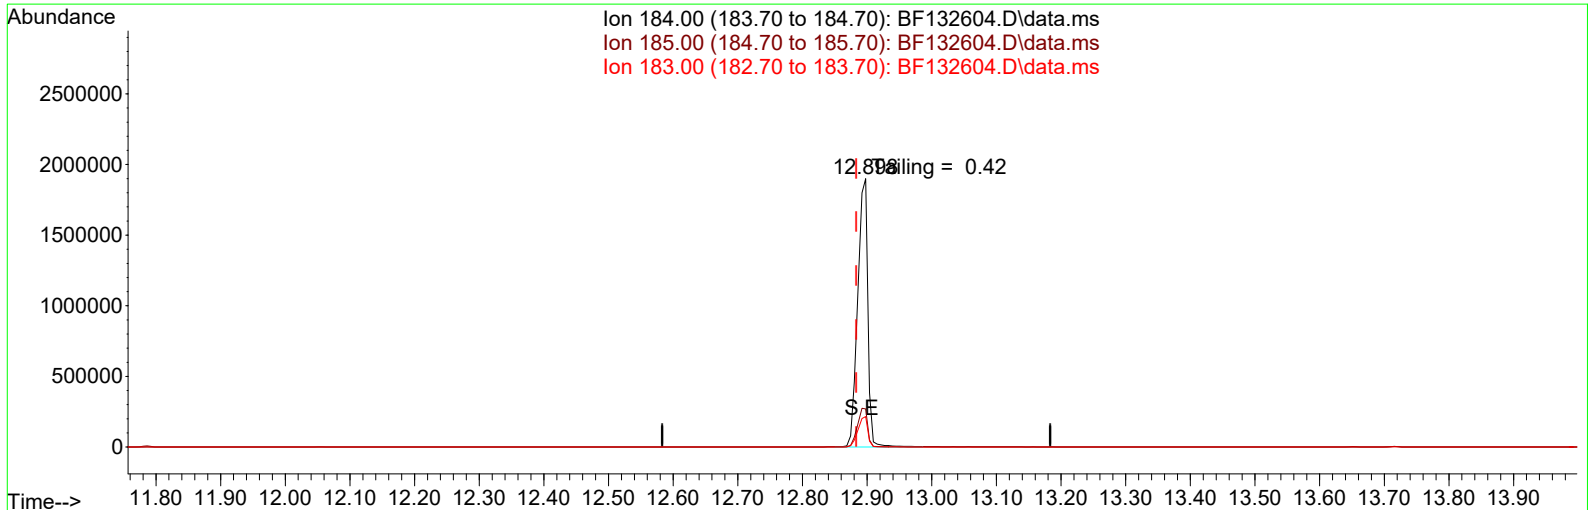

TIC: BF132604.D\data.ms

(77) Benzidine

12.898min (+ 0.015) 77579.45 ng

response 2092464

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.22
183.00	10.90	11.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/2/2023	BNA_F	<u>BF132604.D</u>
Compound Name	Response	Retention Time
DDT	1011878	13.715
DDD	19494	13.445
DDE	1464	13.074
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20958	1032836	2.03

Instrument :
BNA_F
ClientSampleId :
DFTPP