
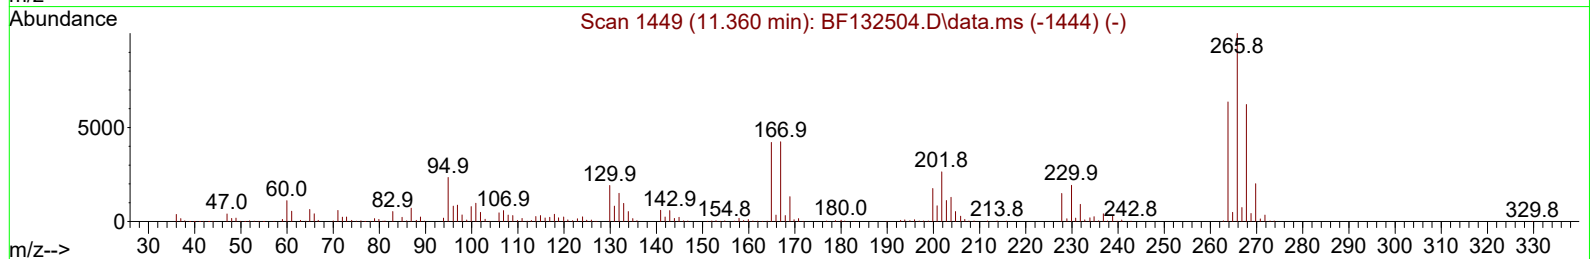
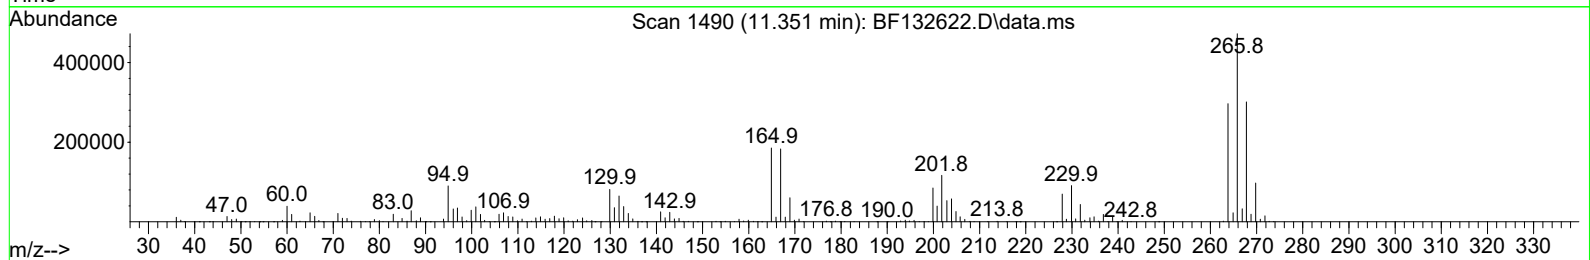


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030323\
Data File : BF132622.D
Acq On : 03 Mar 2023 11:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 03:49:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

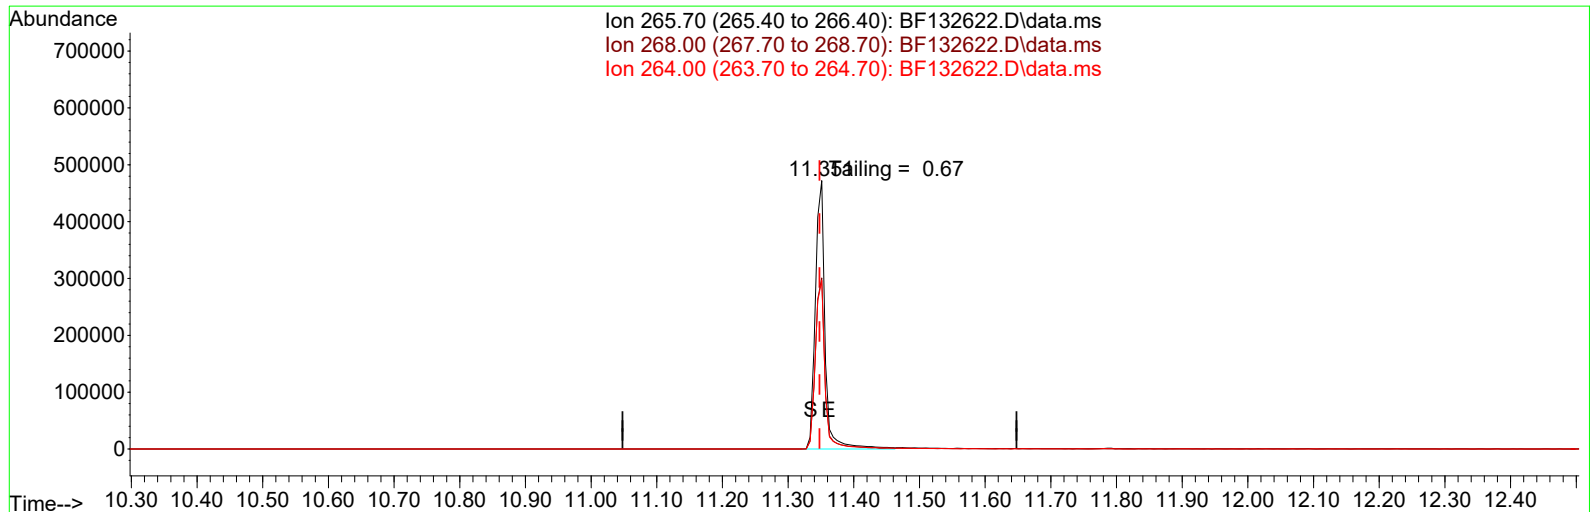

TIC: BF132622.D\data.ms

(70) Pentachlorophenol (C)




11.351min (+ 0.003) 496608.26 ng

response 488826

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.75
264.00	63.60	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030323\
Data File : BF132622.D
Acq On : 03 Mar 2023 11:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 03:49:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

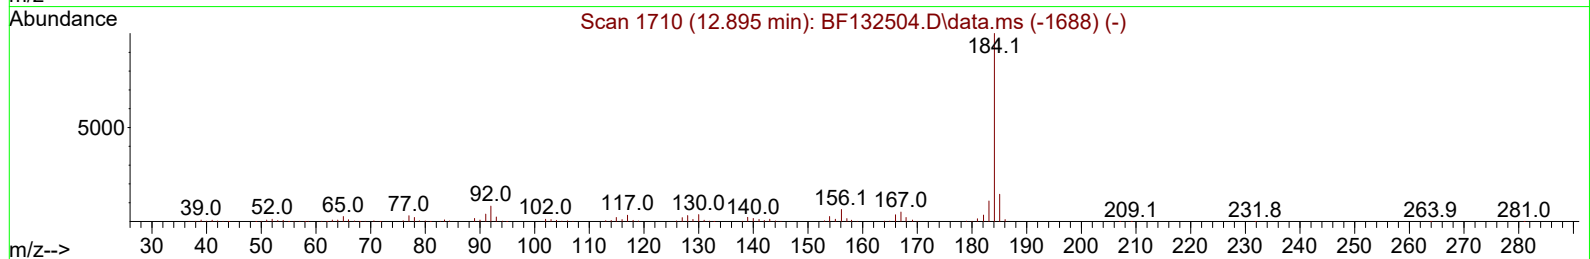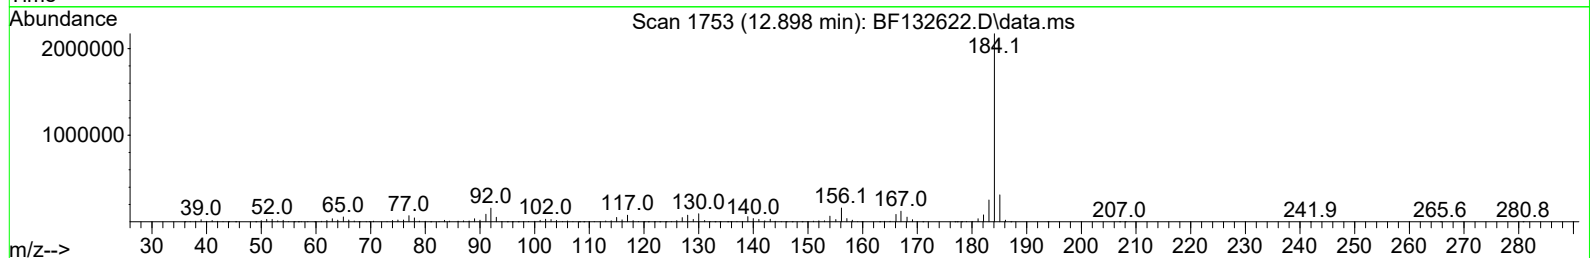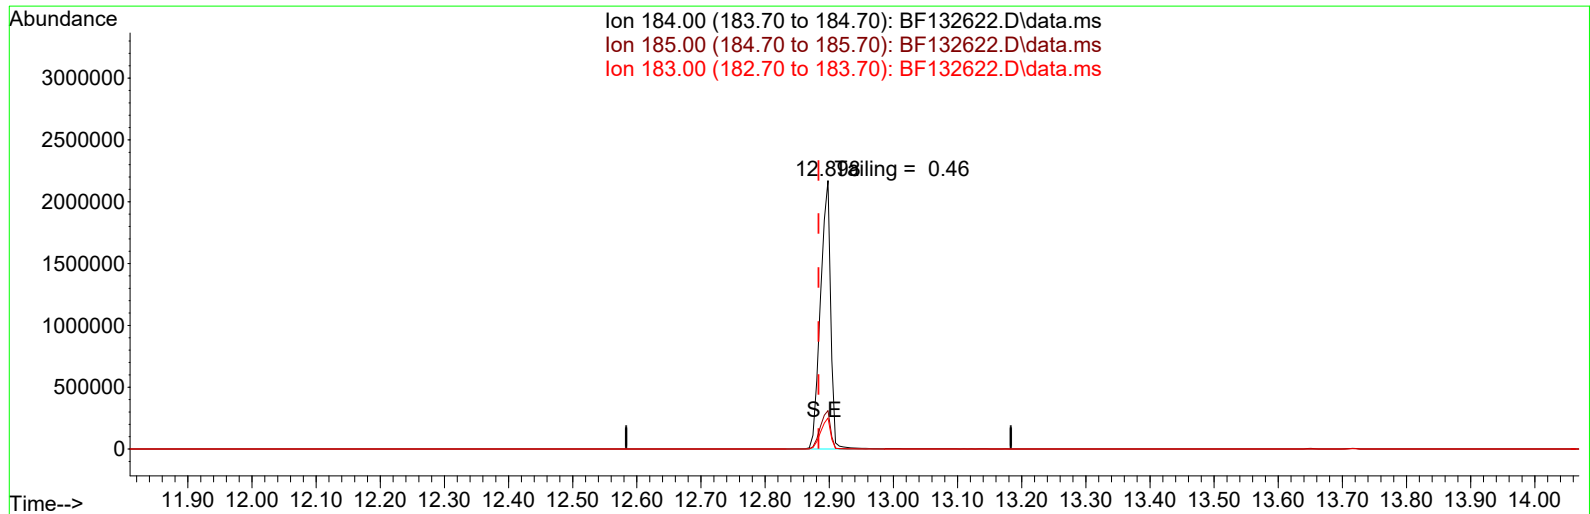

TIC: BF132622.D\data.ms

(77) Benzidine**12.898min (+ 0.015) 117836.96 ng****response 2415267**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.34
183.00	10.90	11.57
0.00	0.00	0.00