
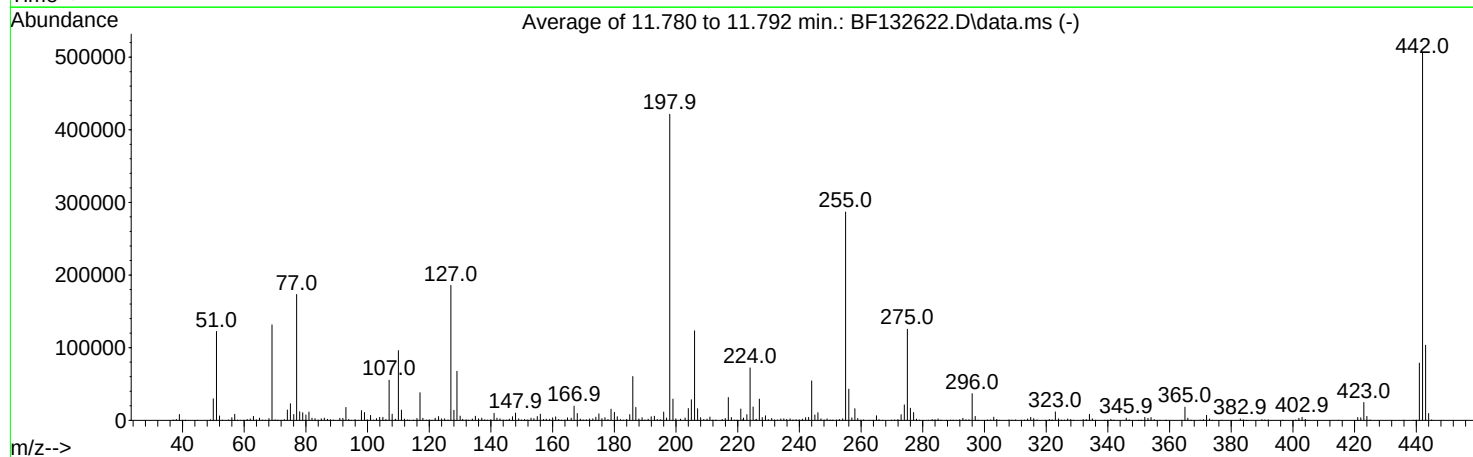


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030323\
 Data File : BF132622.D
 Acq On : 03 Mar 2023 11:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 24 23:17:30 2023

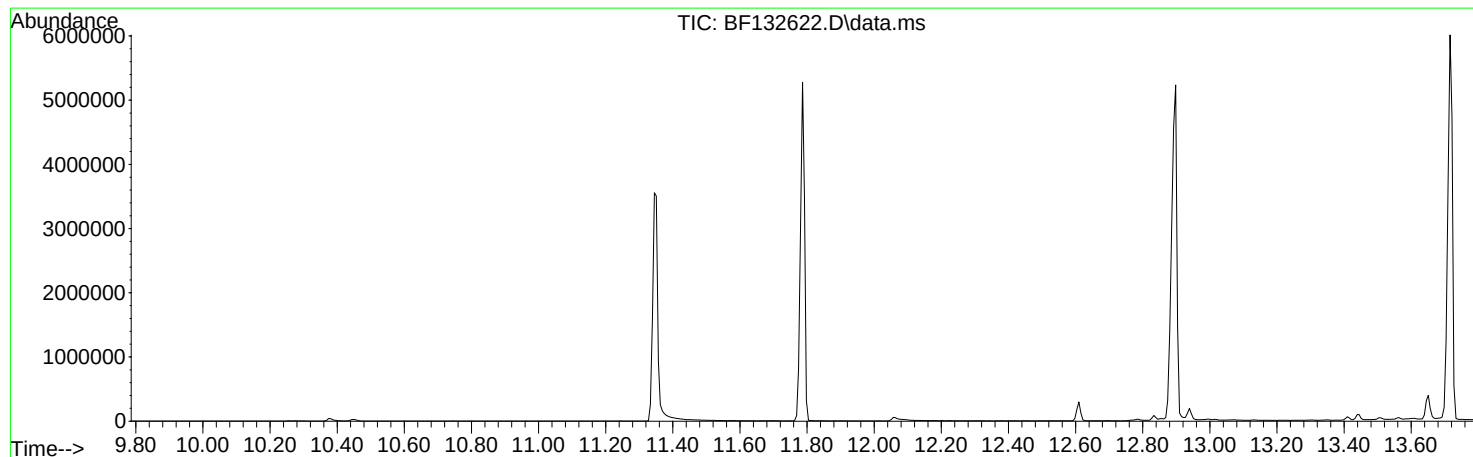




AutoFind: Scans 1563, 1564, 1565; Background Corrected with Scan 1557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	122360	PASS
68	69	0.00	2	1.8	2353	PASS
69	198	0.00	100	31.2	131357	PASS
70	69	0.00	2	0.5	700	PASS
127	198	10	80	44.1	185776	PASS
197	198	0.00	2	0.8	3267	PASS
198	198	100	100	100.0	421227	PASS
199	198	5	9	6.9	29205	PASS
275	198	10	60	29.8	125437	PASS
365	198	1	100	4.3	18122	PASS
441	198	0.01	100	18.7	78808	PASS
442	442	50	100	100.0	506475	PASS
443	442	15	24	20.4	103416	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030323\
 Data File : BF132622.D
 Acq On : 03 Mar 2023 11:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 04 03:49:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 23:17:30 2023
 Response via : Initial Calibration

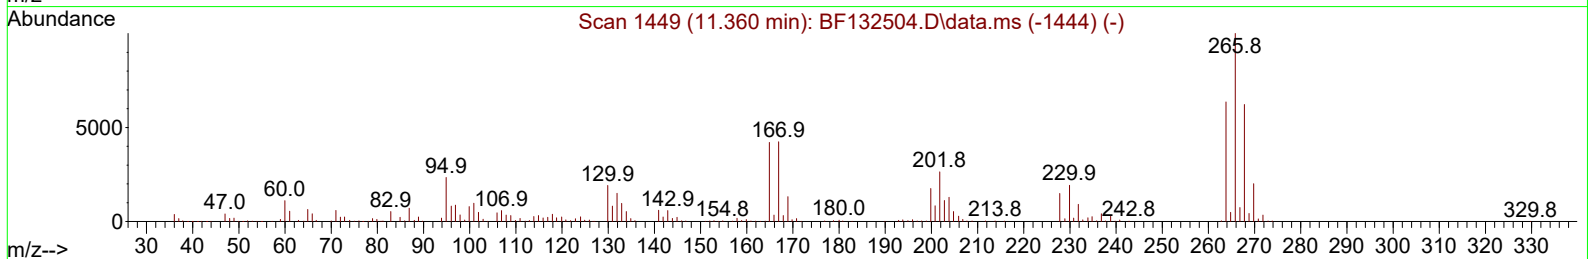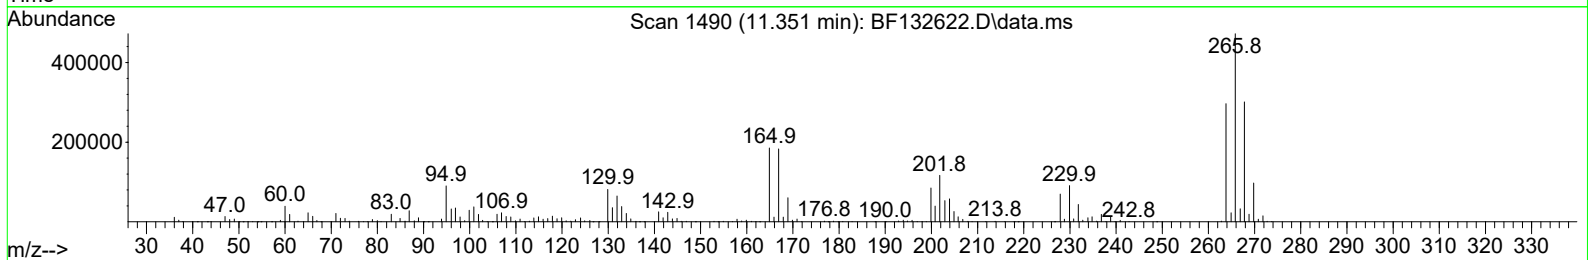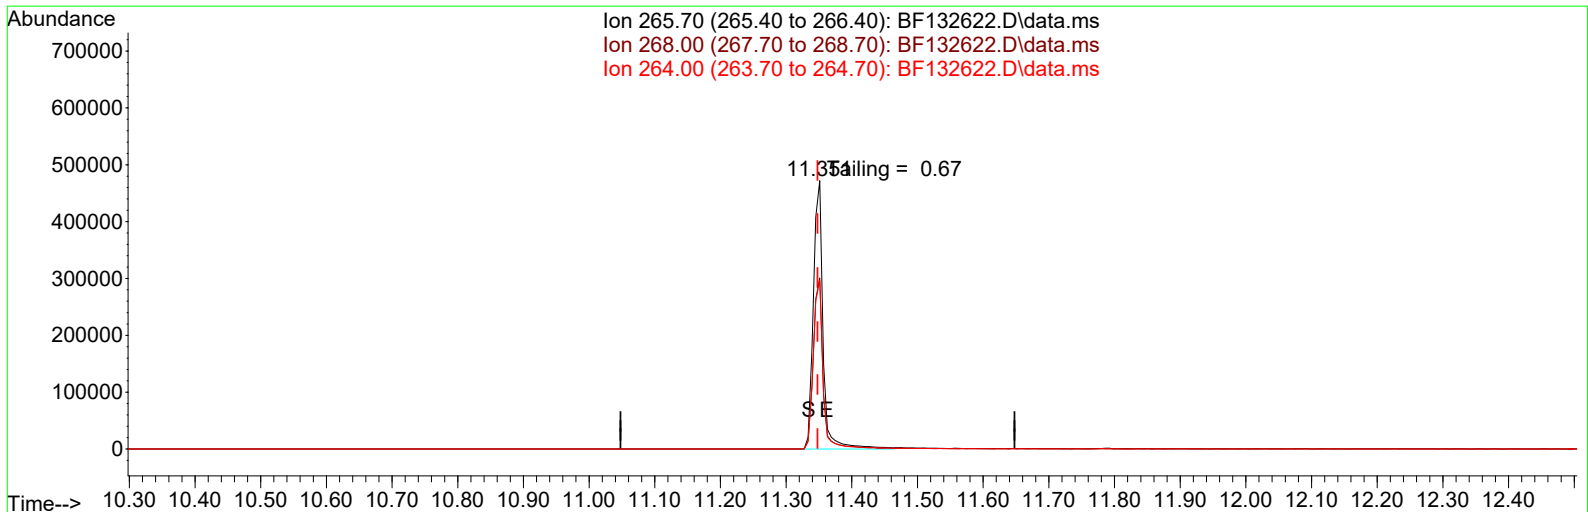

TIC: BF132622.D\data.ms

(70) Pentachlorophenol (C)

11.351min (+ 0.003) 496608.26 ng




response 488826

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.75
264.00	63.60	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030323\
Data File : BF132622.D
Acq On : 03 Mar 2023 11:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 04 03:49:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 23:17:30 2023
Response via : Initial Calibration

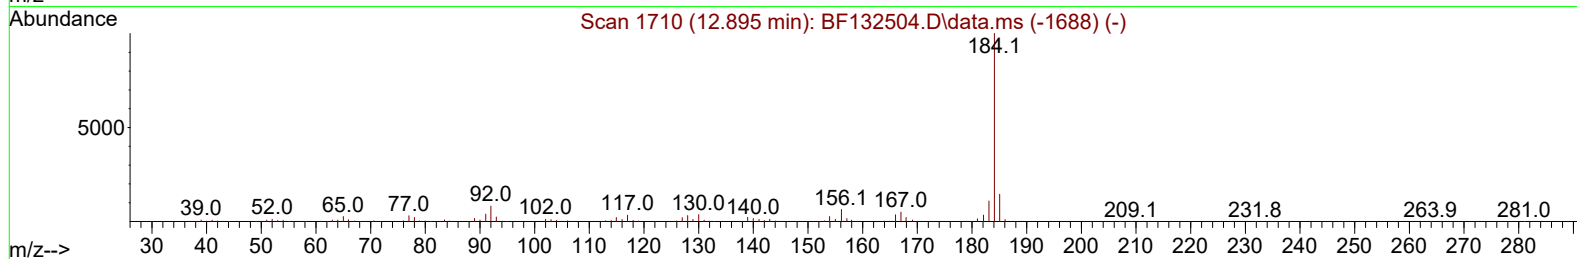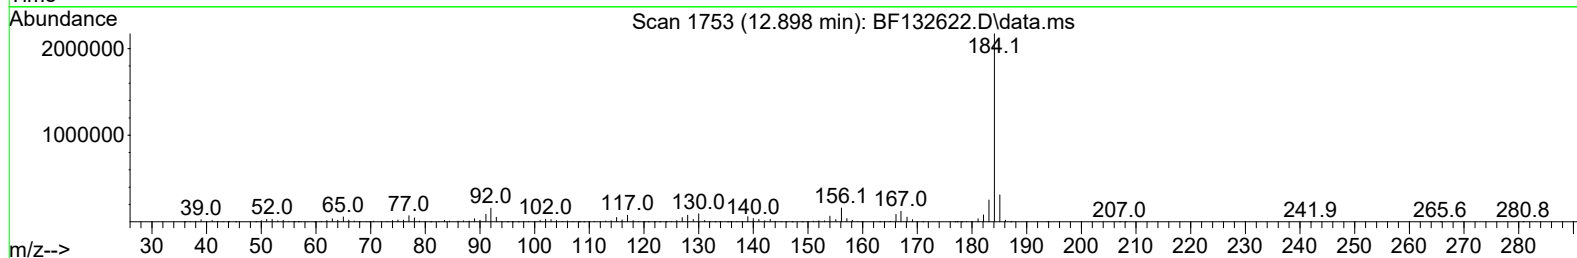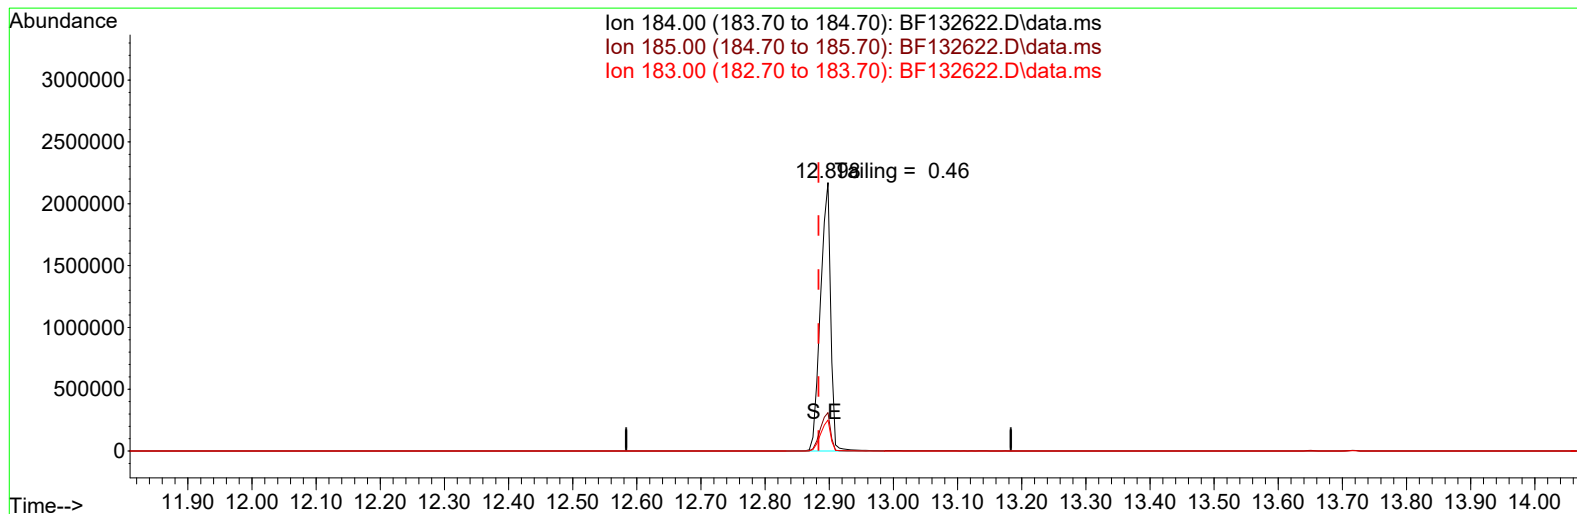

TIC: BF132622.D\data.ms

(77) Benzidine

12.898min (+ 0.015) 117836.96 ng

response 2415267

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.34
183.00	10.90	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/3/2023	BNA_F	<u>BF132622.D</u>
Compound Name	Response	Retention Time
DDT	1179698	13.716
DDD	24727	13.445
DDE	1843	13.074
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26570	1206268	2.20

Instrument :
BNA_F
ClientSampleId :
DFTPP