

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030520\
 Data File : BF119222.D
 Acq On : 5 Mar 2020 20:03
 Operator : CG/JU
 Sample : PB127285BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB127285BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.946	482	486	505	rBV	343206	548395	9.72%	1.650%
2	5.369	554	558	589	rBV	3300325	3500263	62.05%	10.530%
3	6.381	725	730	751	rBV	3075739	3454318	61.24%	10.392%
4	6.722	784	788	798	rBV	878837	775311	13.74%	2.332%
5	6.881	810	815	818	rBV	3215679	3108442	55.11%	9.352%
6	7.287	879	884	900	rBV	1924335	2362439	41.88%	7.107%
7	8.004	1001	1006	1025	rBV	1040072	1038459	18.41%	3.124%
8	9.081	1183	1189	1192	rBV	4433536	4959061	87.91%	14.919%
9	9.757	1298	1304	1321	rBB	1370308	1315004	23.31%	3.956%
10	10.551	1434	1439	1463	rBV	3358134	3370874	59.76%	10.141%
11	11.239	1553	1556	1565	rBV	1456072	1364362	24.19%	4.105%
12	12.827	1821	1826	1829	rBV	5639049	5640791	100.00%	16.970%
13	13.880	2001	2005	2019	rBV	1083434	1003941	17.80%	3.020%
14	15.304	2243	2247	2261	rBV	587562	798166	14.15%	2.401%


Sum of corrected areas: 33239826

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF030520\
Data File : BF119222.D
Acq On : 5 Mar 2020 20:03
Operator : CG/JU
Sample : PB127285BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127285BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

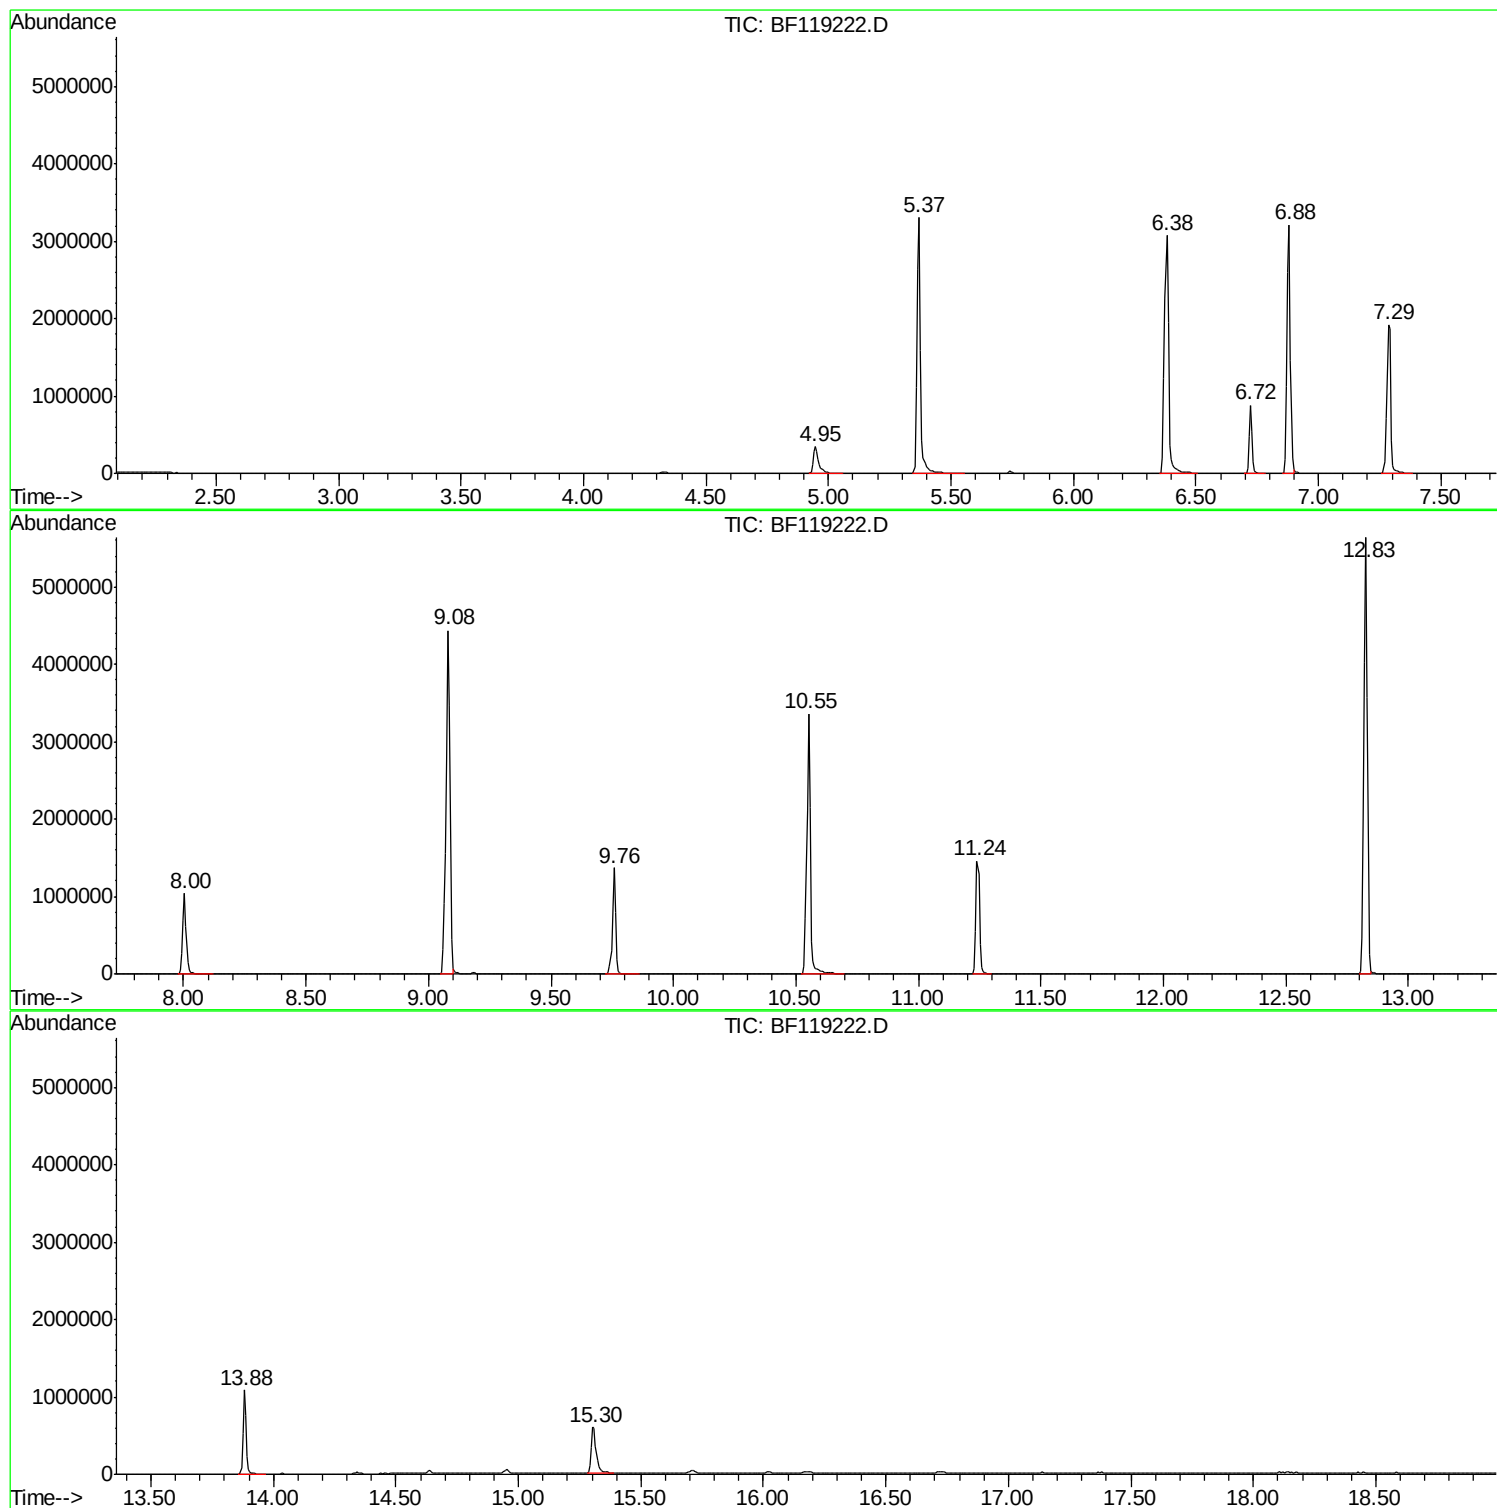

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF030520\
Data File : BF119222.D
Acq On : 5 Mar 2020 20:03
Operator : CG/JU
Sample : PB127285BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127285BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.95	14.15 ng	548395	1,4-Dichlorobenzene-d4	6.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		(+)-4-Amino-4,5-dihydro-2(3H)-furanone	101	C4H7NO2	016504-58-8	47
3		Guanidine	59	CH5N3	000113-00-8	43
4		Acetic acid, cyano-, 1,1-dimethyl-	141	C7H11NO2	001116-98-9	25
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

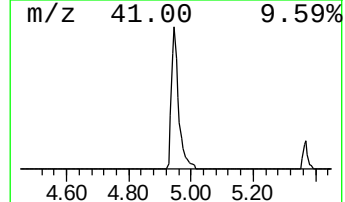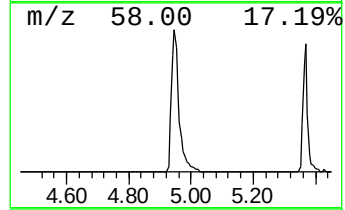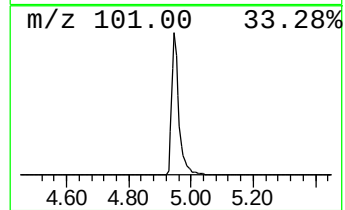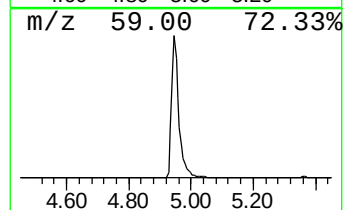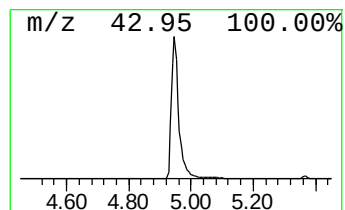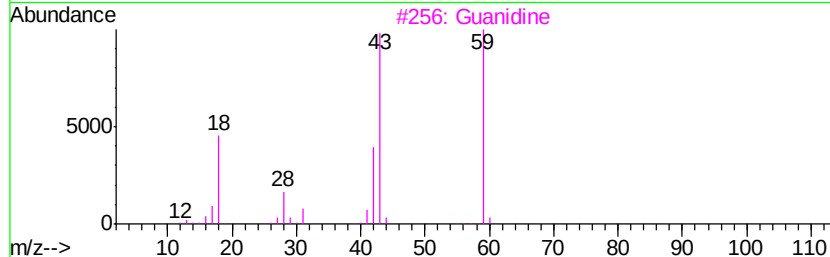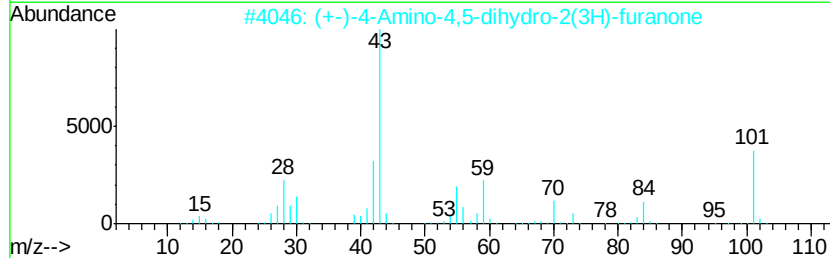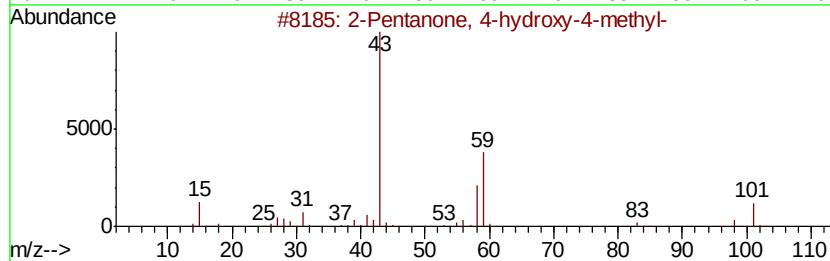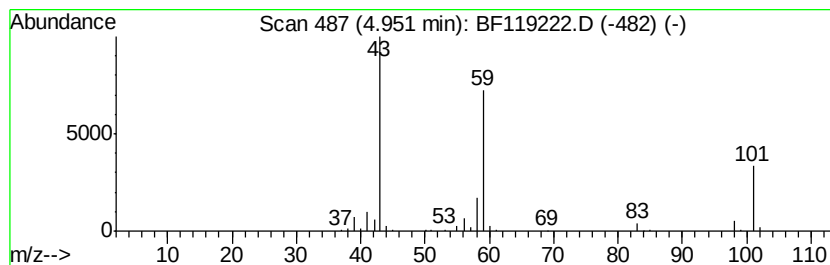

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030520\
Data File : BF119222.D
Acq On : 5 Mar 2020 20:03
Operator : CG/JU
Sample : PB127285BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127285BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.95	14.2	ng	548395	1	6.72	775311	20.0