


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030520\
 Data File : BF119241.D
 Acq On : 6 Mar 2020 6:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 26 16:03:05 2020

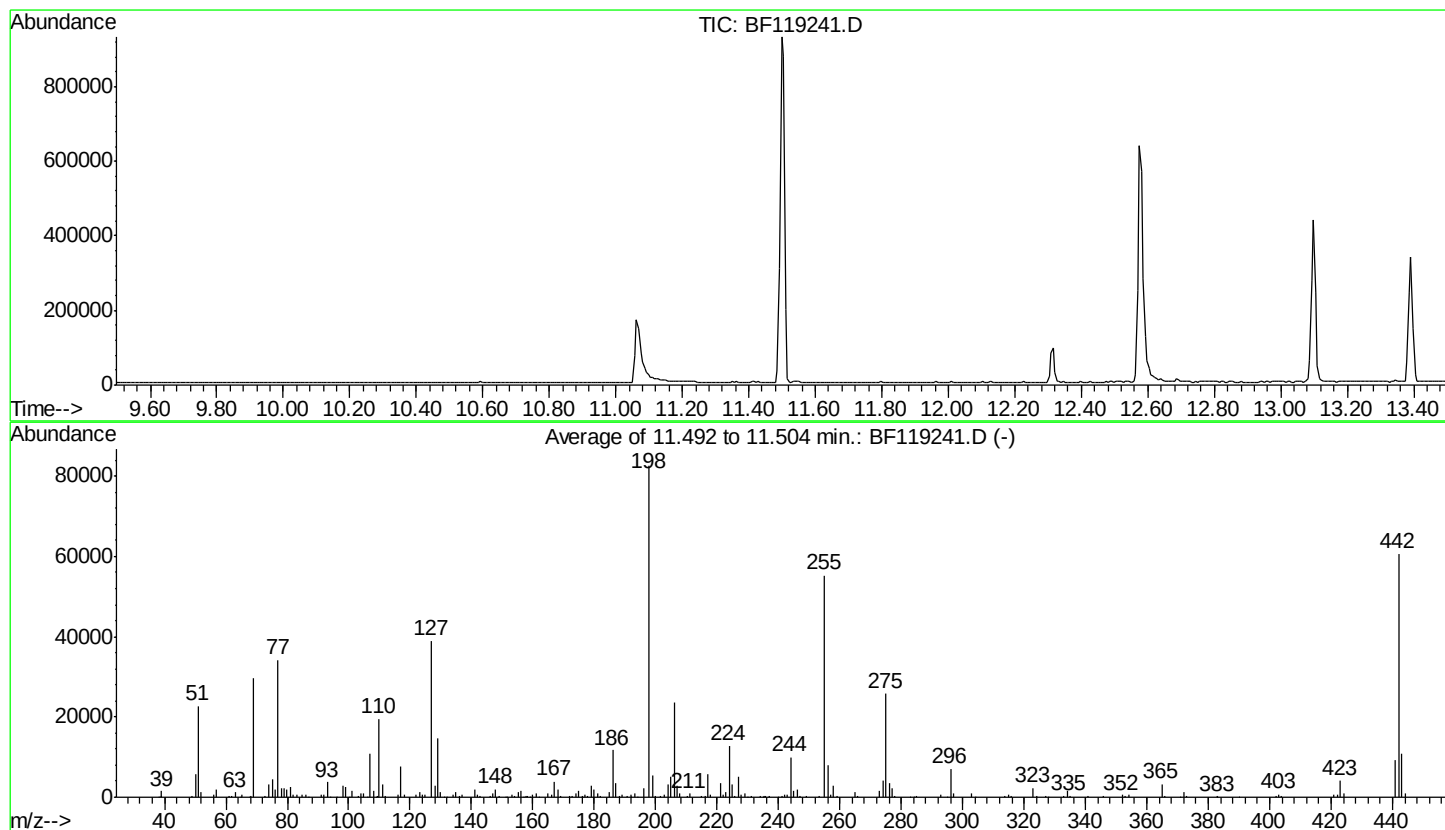

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	22802	PASS
68	69	0.00	2	0.9	256	PASS
69	198	0.00	100	35.9	29664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	39074	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82621	PASS
199	198	5	9	6.8	5584	PASS
275	198	10	60	31.2	25749	PASS
365	198	1	100	4.0	3272	PASS
441	198	0.01	100	11.3	9316	PASS
442	198	50	100	73.4	60616	PASS
443	442	15	24	18.2	11012	PASS