

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030719\
 Data File : BG039808.D
 Acq On : 7 Mar 2019 18:47
 Operator : JU/SJ
 Sample : PB117706TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB117706TB

Quant Time: Mar 07 23:53:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	40184	20.00	ng	-0.02
21) Naphthalene-d8	10.98	136	173705	20.00	ng	-0.01
39) Acenaphthene-d10	14.78	164	121661	20.00	ng	-0.01
64) Phenanthrene-d10	17.52	188	313120	20.00	ng	-0.01
76) Chrysene-d12	21.81	240	330435	20.00	ng	-0.02
87) Perylene-d12	25.18	264	324425	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.70	112	352087	149.48	ng	-0.01
7) Phenol-d6	7.30	99	513929	146.33	ng	-0.01
23) Nitrobenzene-d5	9.33	82	295674	92.06	ng	-0.01
42) 2,4,6-Tribromophenol	16.26	330	202574	142.85	ng	-0.01
45) 2-Fluorobiphenyl	13.40	172	774378	90.63	ng	-0.01
79) Terphenyl-d14	20.12	244	1302177	86.77	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.33	70	38989	15.423	ng	# 68
51) 2,6-Dinitrotoluene	14.78	165	15854	7.351	ng	# 25
57) 2,4-Dinitrotoluene	14.78	165	15854	5.232	ng	# 20
67) 4-Bromophenyl-phenylether	16.26	248	15948	4.550	ng	# 1
77) Benzidine	20.12	184	22421	2.138	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030719\
Data File : BG039808.D
Acq On : 7 Mar 2019 18:47
Operator : JU/SJ
Sample : PB117706TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB117706TB

Quant Time: Mar 07 23:53:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

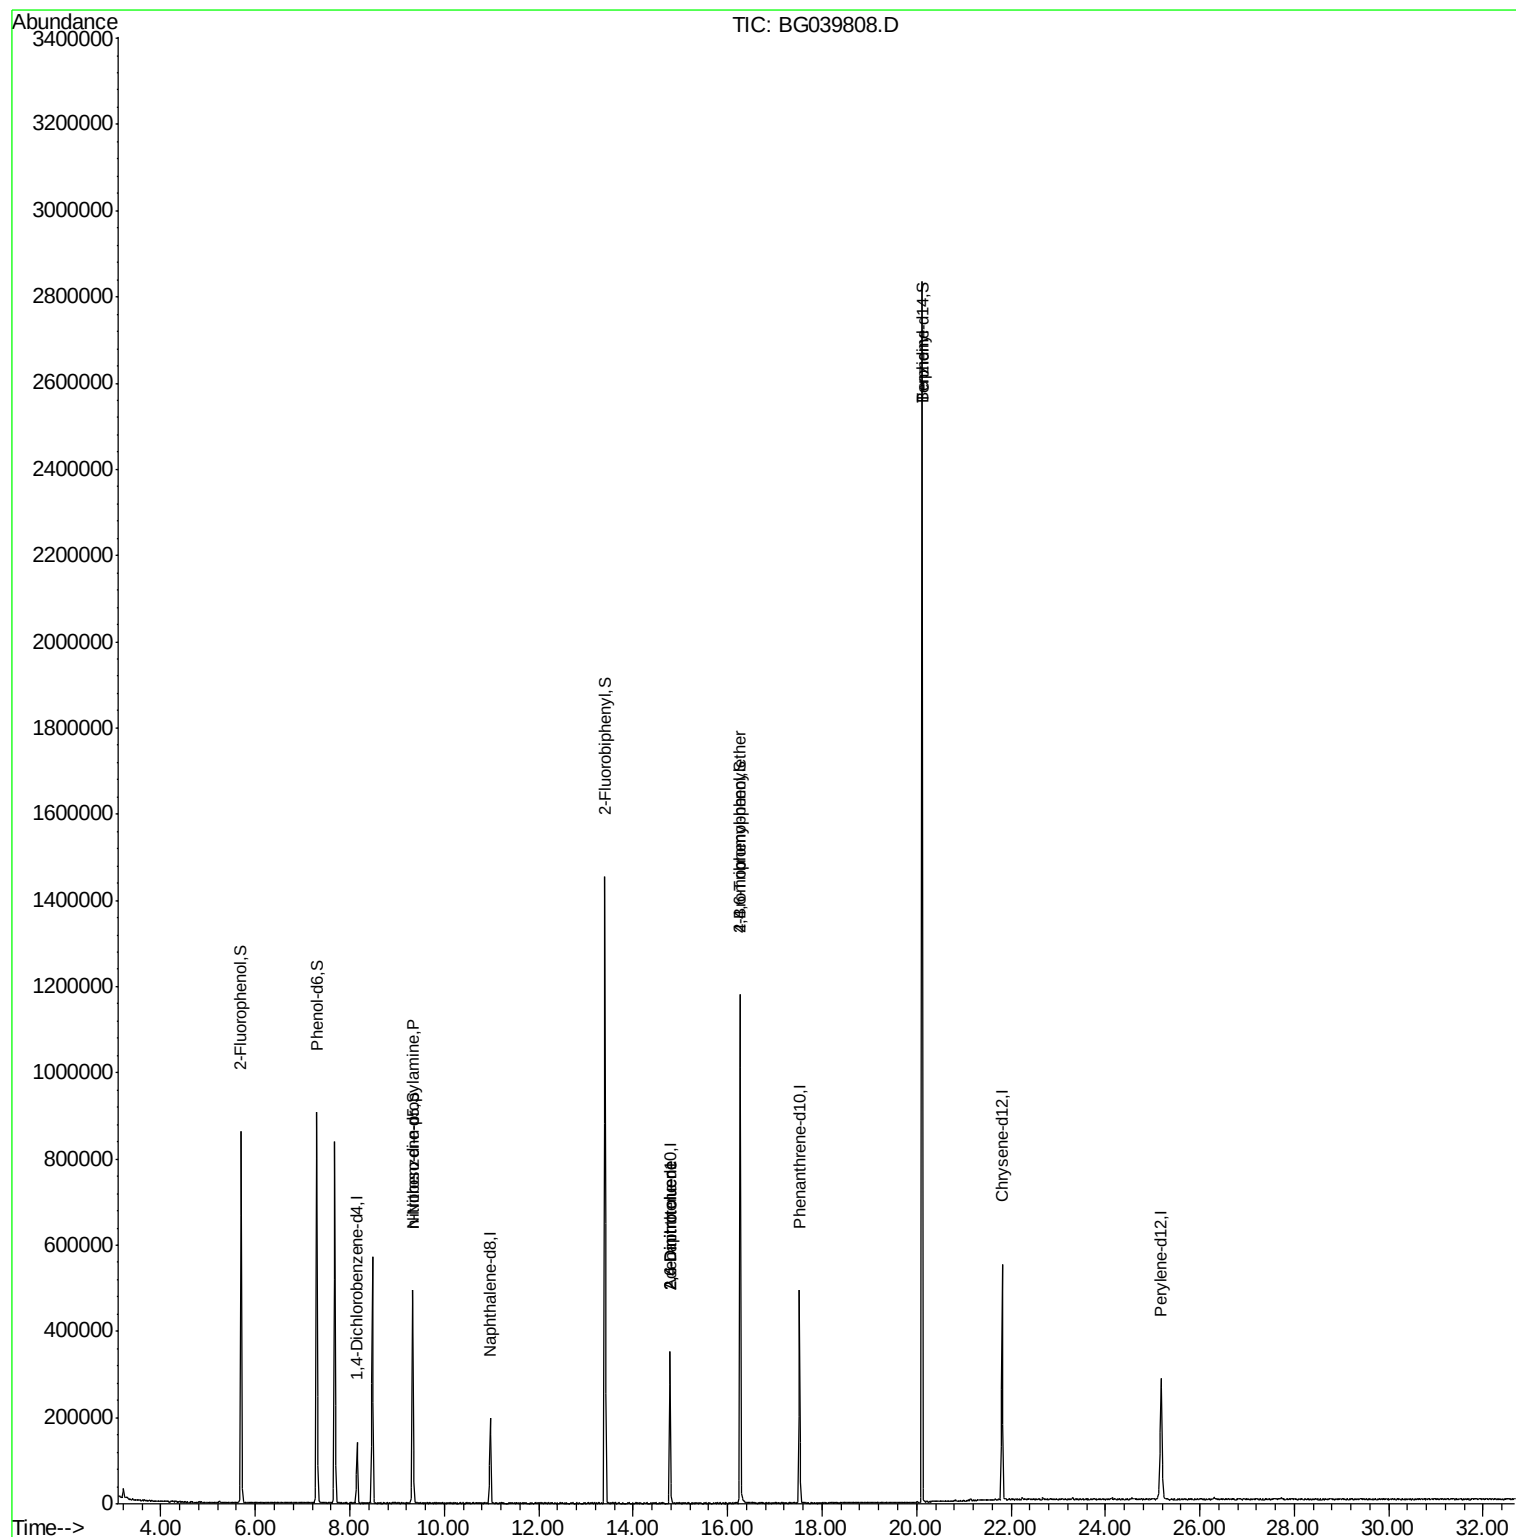




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.15 min Scan# 862
Delta R.T. -0.02 min
Lab File: BG039808.D
Acq: 7 Mar 2019 18:47

Instrument :
BNA_F
ClientSampleId :
PB117706TB

Tgt Ion:152 Resp: 40184
Ion Ratio Lower Upper
152 100
150 151.9 123.7 185.5
115 61.9 45.9 68.9

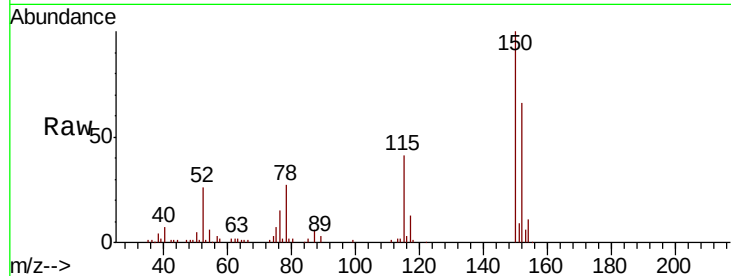


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

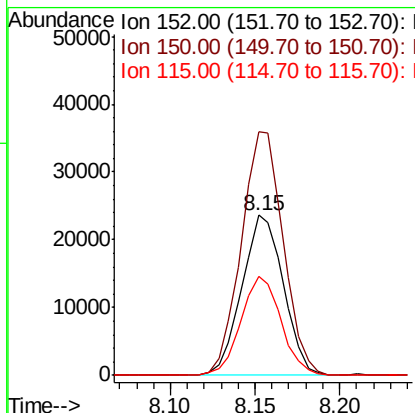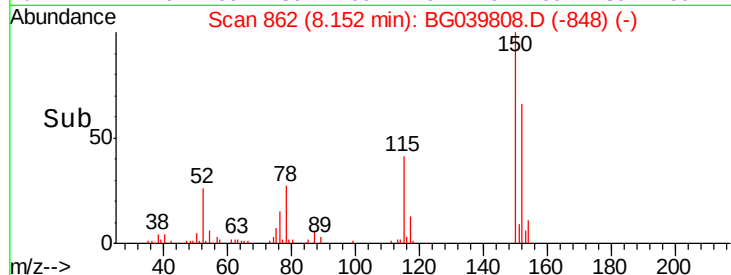



#5


2-Fluorophenol
Concen: 149.478 ng
RT: 5.70 min Scan# 444
Delta R.T. -0.01 min
Lab File: BG039808.D
Acq: 7 Mar 2019 18:47

Tgt Ion:112 Resp: 352087
Ion Ratio Lower Upper
112 100
64 71.7 57.8 86.8
63 36.5 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

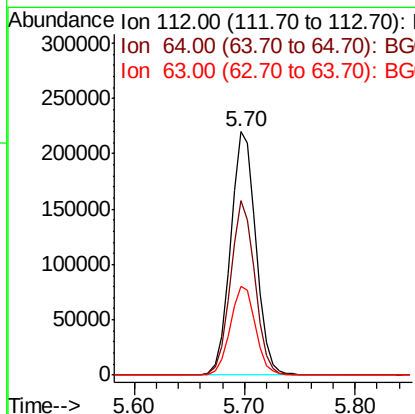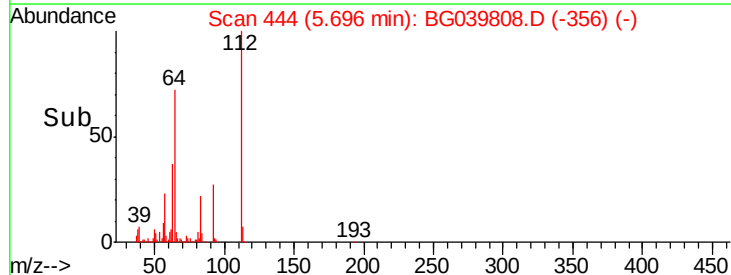



#7

Phenol-d6

Concen: 146.331 ng

RT: 7.30 min Scan# 717

Delta R.T. -0.01 min

Lab File: BG039808.D

Acq: 7 Mar 2019 18:47

Instrument :

BNA_F

ClientSampleId :

PB117706TB


Tgt Ion: 99 Resp: 513929

Ion Ratio Lower Upper




99 100

42 20.3 18.2 27.2

71 35.9 28.0 42.0

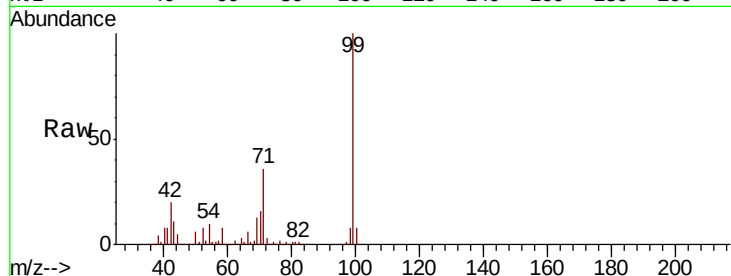

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

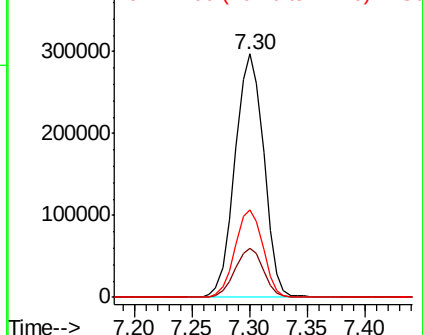

#19

n-Nitroso-di-n-propylamine

Concen: 15.423 ng

RT: 9.33 min Scan# 1063

Delta R.T. 0.36 min

Lab File: BG039808.D

Acq: 7 Mar 2019 18:47

Tgt Ion: 70 Resp: 38989


Ion Ratio Lower Upper

70 100



42 49.5 60.4 90.6#


101 0.0 7.5 11.3#

130 1.7 16.9 25.3#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

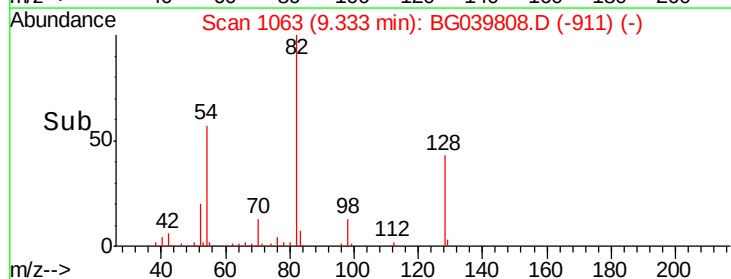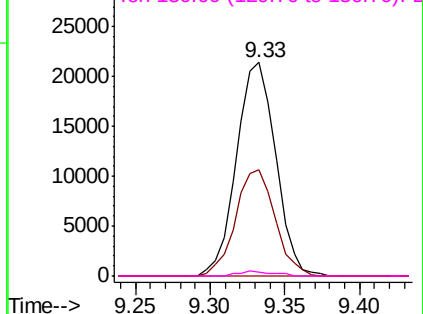


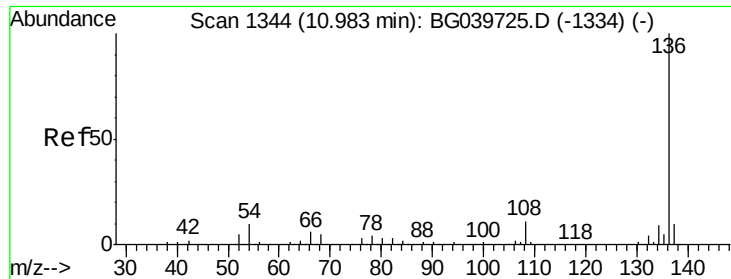




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.98 min Scan# 1343
Delta R.T. -0.01 min
Lab File: BG039808.D
Acq: 7 Mar 2019 18:47

Instrument :
BNA_F
ClientSampleId :
PB117706TB

Tgt Ion:	136	Resp:	173705
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.1	13.7
54	10.4	9.4	14.2
68	5.6	4.2	6.4




Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

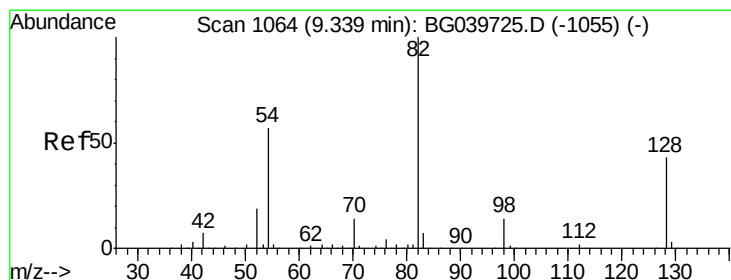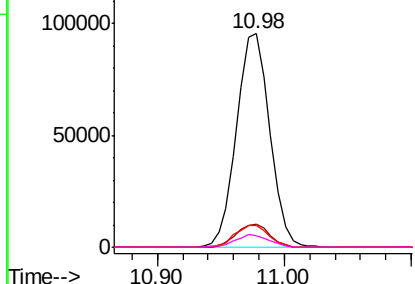




#23
Nitrobenzene-d5
Concen: 92.060 ng
RT: 9.33 min Scan# 1063
Delta R.T. -0.01 min
Lab File: BG039808.D
Acq: 7 Mar 2019 18:47

Tgt Ion:	82	Resp:	295674
Ion	Ratio	Lower	Upper
82	100		
128	43.2	31.3	46.9
54	57.0	50.9	76.3



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

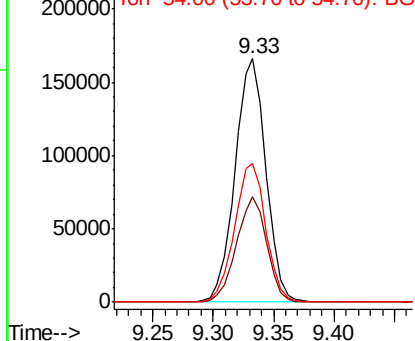

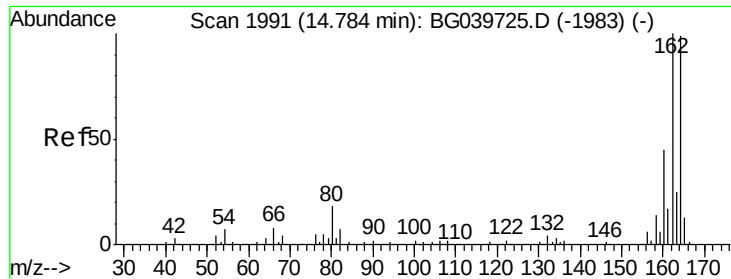

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.78 min Scan# 1990

Delta R.T. -0.01 min

Lab File: BG039808.D

Acq: 7 Mar 2019 18:47

Instrument :

BNA_F

ClientSampleId :

PB117706TB


Tgt Ion:164 Resp: 121661

Ion Ratio Lower Upper

164 100

162 104.0 81.6 122.4




160 43.9 34.2 51.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

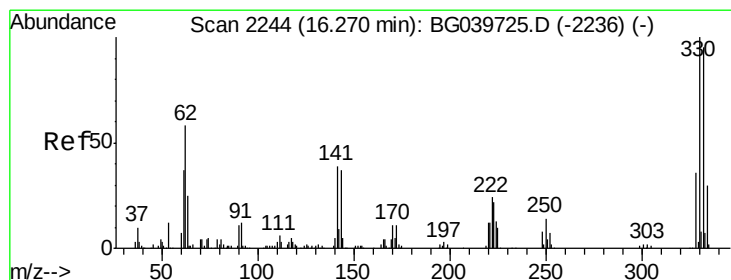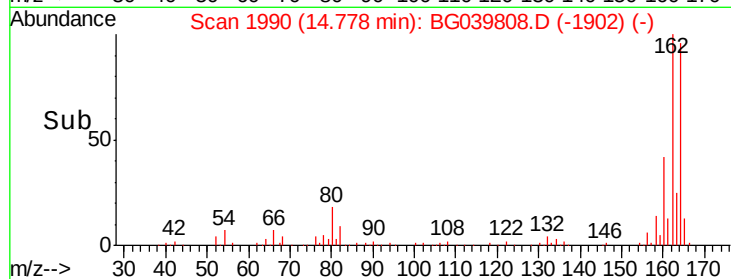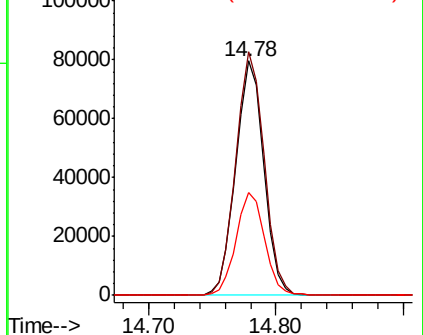

#42

2,4,6-Tribromophenol

Concen: 142.854 ng

RT: 16.26 min Scan# 2243

Delta R.T. -0.01 min

Lab File: BG039808.D

Acq: 7 Mar 2019 18:47


Tgt Ion:330 Resp: 202574

Ion Ratio Lower Upper

330 100

332 96.4 75.7 113.5



141 41.6 35.6 53.4

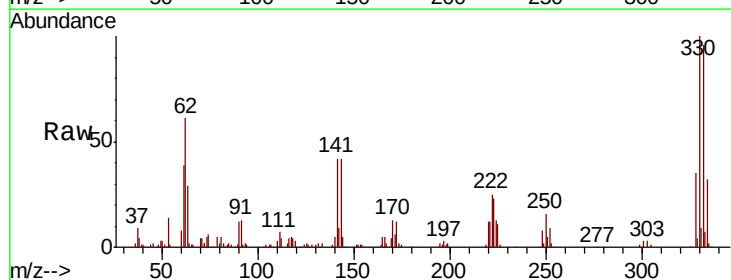


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

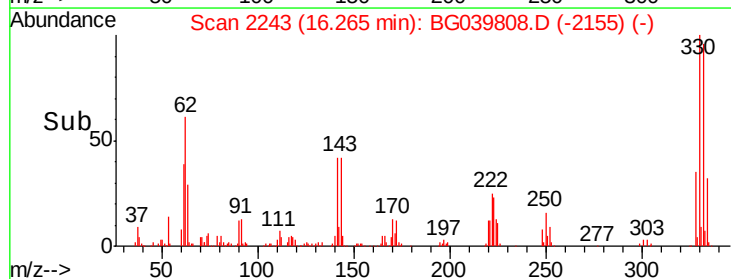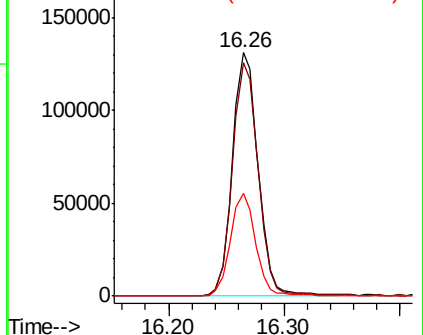







#45
 2-Fluorobiphenyl
 Concen: 90.627 ng
 RT: 13.40 min Scan# 1756
 Delta R.T. -0.01 min
 Lab File: BG039808.D
 Acq: 7 Mar 2019 18:47

Instrument :
 BNA_F
 ClientSampleId :
 PB117706TB

Tgt Ion:172 Resp: 774378
 Ion Ratio Lower Upper
 172 100
 171 37.5 30.8 46.2
 170 25.0 20.2 30.4




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


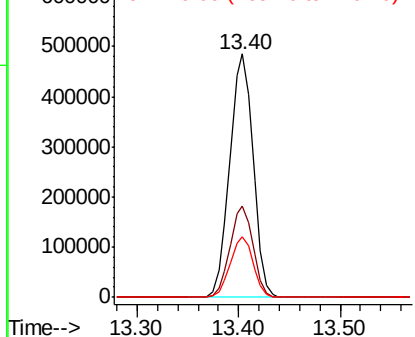



#51
 2,6-Dinitrotoluene
 Concen: 7.351 ng
 RT: 14.78 min Scan# 1990
 Delta R.T. 0.41 min
 Lab File: BG039808.D
 Acq: 7 Mar 2019 18:47

Tgt Ion:165 Resp: 15854
 Ion Ratio Lower Upper
 165 100
 63 2.2 47.0 70.6#
 89 2.3 45.8 68.8#



Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC




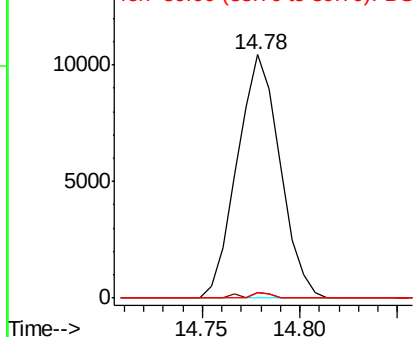


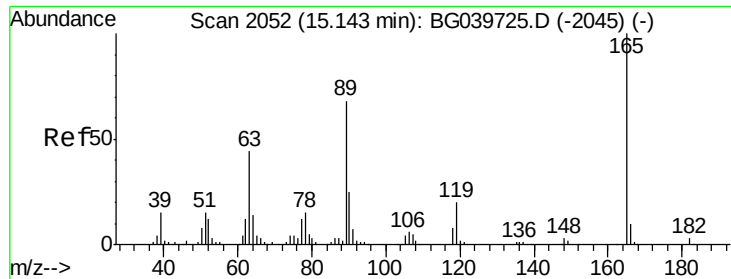

#57
 2,4-Dinitrotoluene
 Concen: 5.232 ng
 RT: 14.78 min Scan# 1990
 Delta R.T. -0.37 min
 Lab File: BG039808.D
 Acq: 7 Mar 2019 18:47




Instrument :
 BNA_F
 ClientSampleId :
 PB117706TB


Tgt Ion:	165	Resp:	15854
Ion	Ratio	Lower	Upper
165	100		
63	2.2	41.0	61.6#
89	2.3	64.6	96.8#
182	0.0	2.0	3.0#

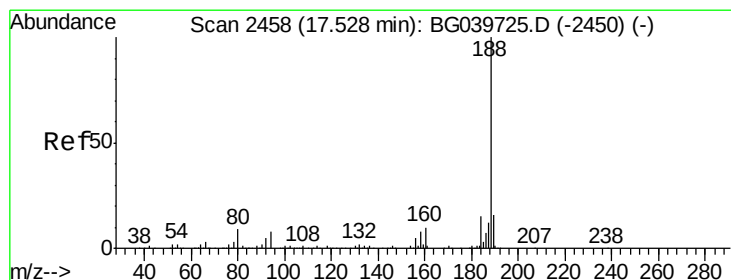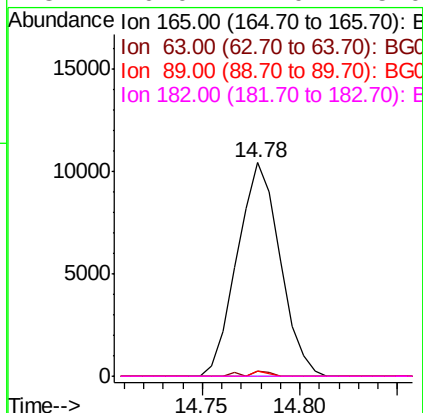

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.52 min Scan# 2457
 Delta R.T. -0.01 min
 Lab File: BG039808.D
 Acq: 7 Mar 2019 18:47

Tgt Ion:	188	Resp:	313120
Ion	Ratio	Lower	Upper
188	100		
94	8.0	6.9	10.3
80	8.7	8.1	12.1

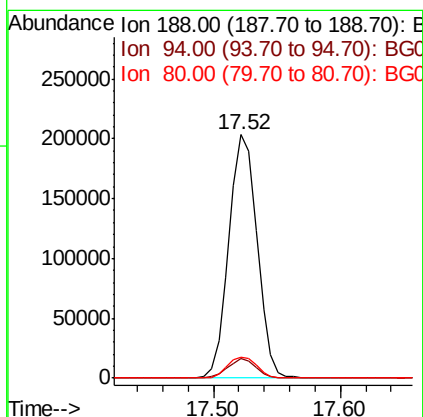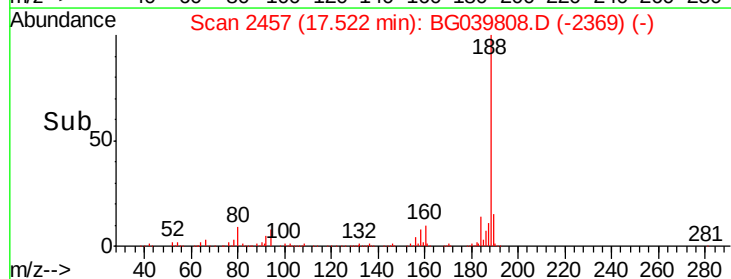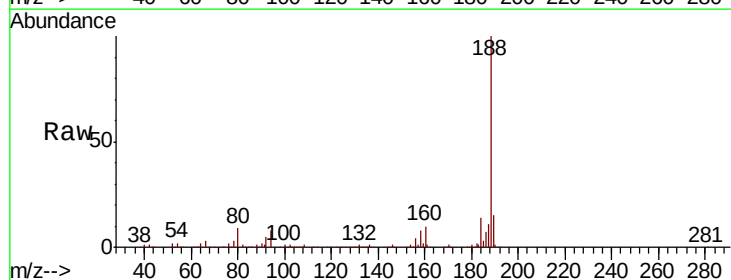


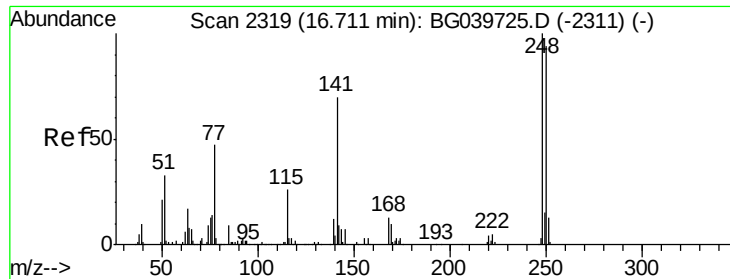




#67
 4-Bromophenyl-phenylether
 Concen: 4.550 ng
 RT: 16.26 min Scan# 2243
 Delta R.T. -0.45 min
 Lab File: BG039808.D
 Acq: 7 Mar 2019 18:47

Instrument :
 BNA_F
 ClientSampleId :
 PB117706TB

Tgt Ion:248 Resp: 15948
 Ion Ratio Lower Upper
 248 100
 250 200.2 77.6 116.4#
 141 521.6 63.9 95.9#

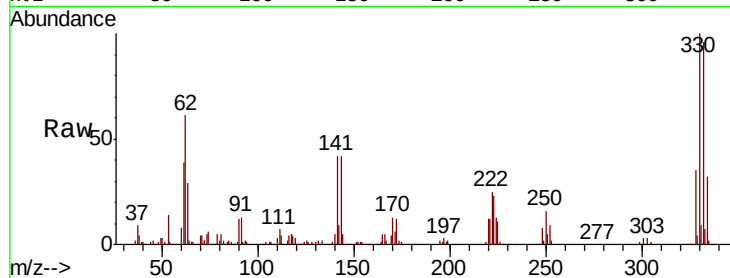


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

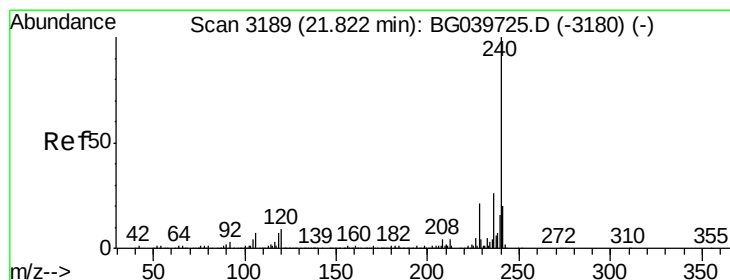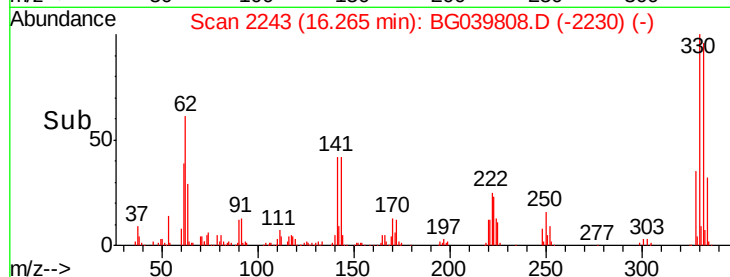
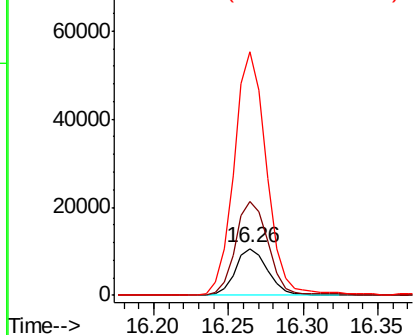



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.81 min Scan# 3187
 Delta R.T. -0.02 min
 Lab File: BG039808.D
 Acq: 7 Mar 2019 18:47

Tgt Ion:240 Resp: 330435
 Ion Ratio Lower Upper
 240 100
 120 9.4 7.0 10.6
 236 25.0 21.0 31.4

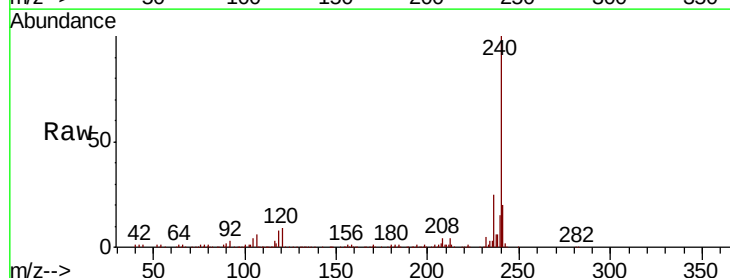

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



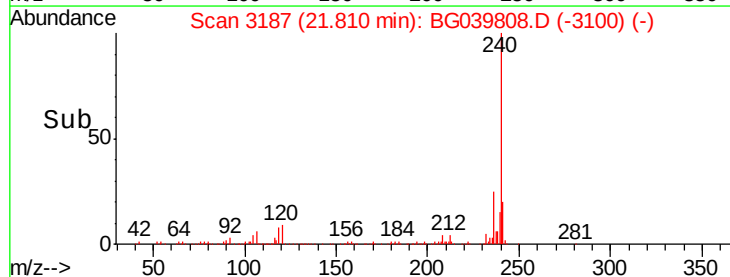
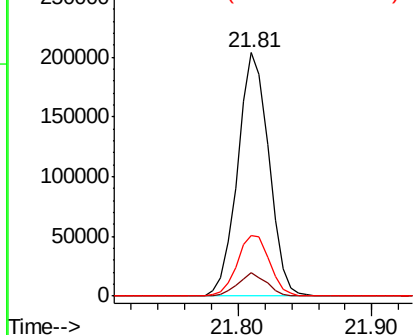




#77
Benzidine
Concen: 2.138 ng
RT: 20.12 min Scan# 2899
Delta R.T. 0.36 min
Lab File: BG039808.D
Acq: 7 Mar 2019 18:47




Instrument :
BNA_F
ClientSampleId :
PB117706TB


Tgt Ion:184 Resp: 22421
Ion Ratio Lower Upper
184 100
185 18.4 12.2 18.2#
183 7.8 10.6 15.8#

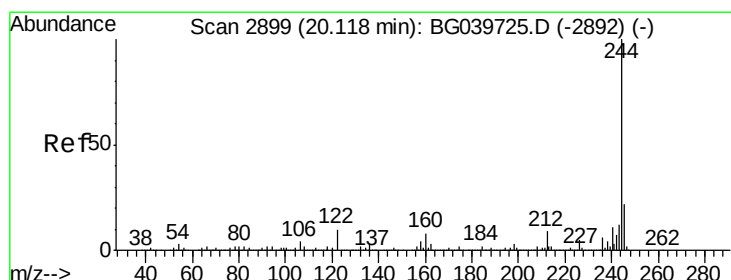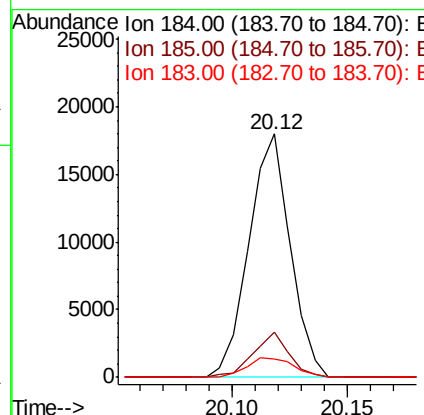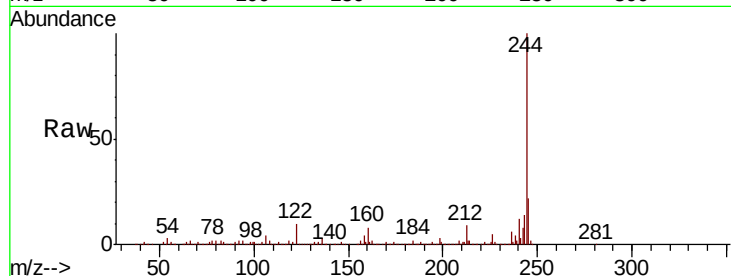

#79
Terphenyl-d14
Concen: 86.769 ng
RT: 20.12 min Scan# 2899
Delta R.T. -0.01 min
Lab File: BG039808.D
Acq: 7 Mar 2019 18:47

Tgt Ion:244 Resp: 1302177
Ion Ratio Lower Upper
244 100
212 9.2 7.3 10.9
122 9.7 8.4 12.6

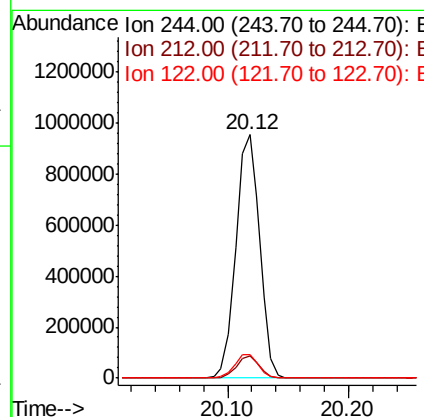

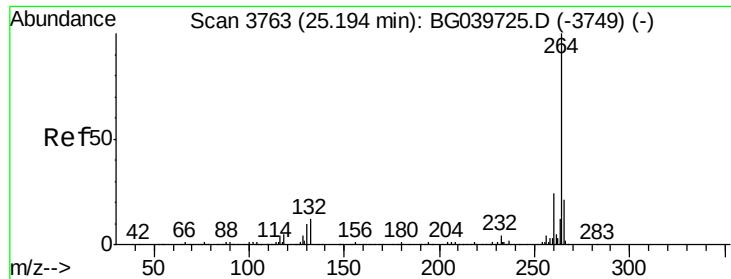

#87
Perylene-d12
Concen: 20.000 ng
RT: 25.18 min Scan# 3761
Delta R.T. -0.02 min
Lab File: BG039808.D
Acq: 7 Mar 2019 18:47

Instrument :
BNA_F
ClientSampleId :
PB117706TB

Tgt Ion: 264 Resp: 324425
Ion Ratio Lower Upper
264 100
260 24.0 18.2 27.4
265 21.9 18.5 27.7

