

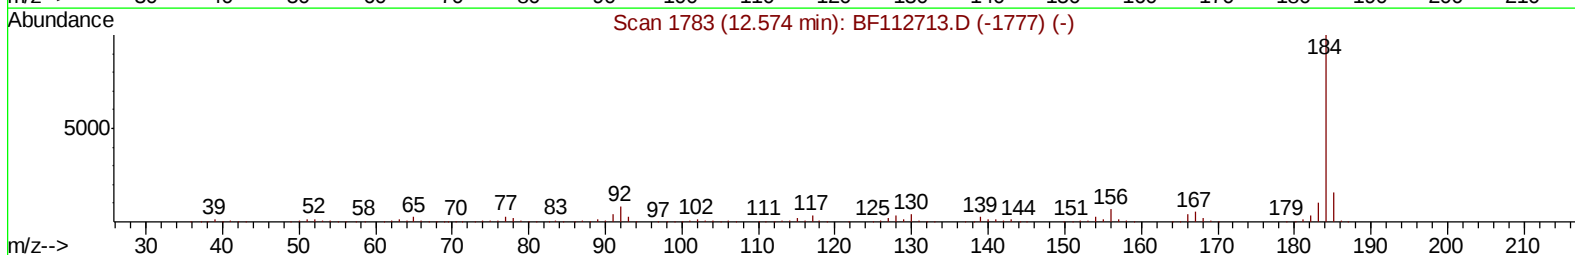


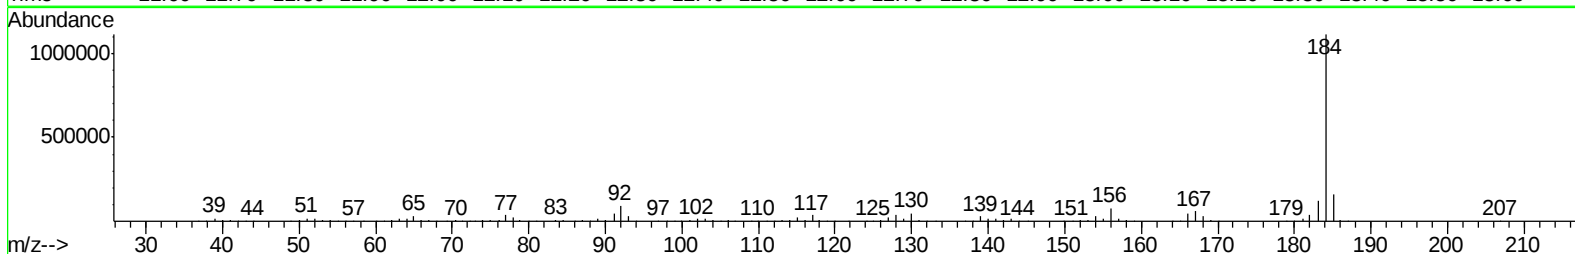

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF030619\  
Data File : BF112880.D  
Acq On : 6 Mar 2019 12:18  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 05:59:59 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF022719.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 01 15:40:43 2019  
Response via : Initial Calibration

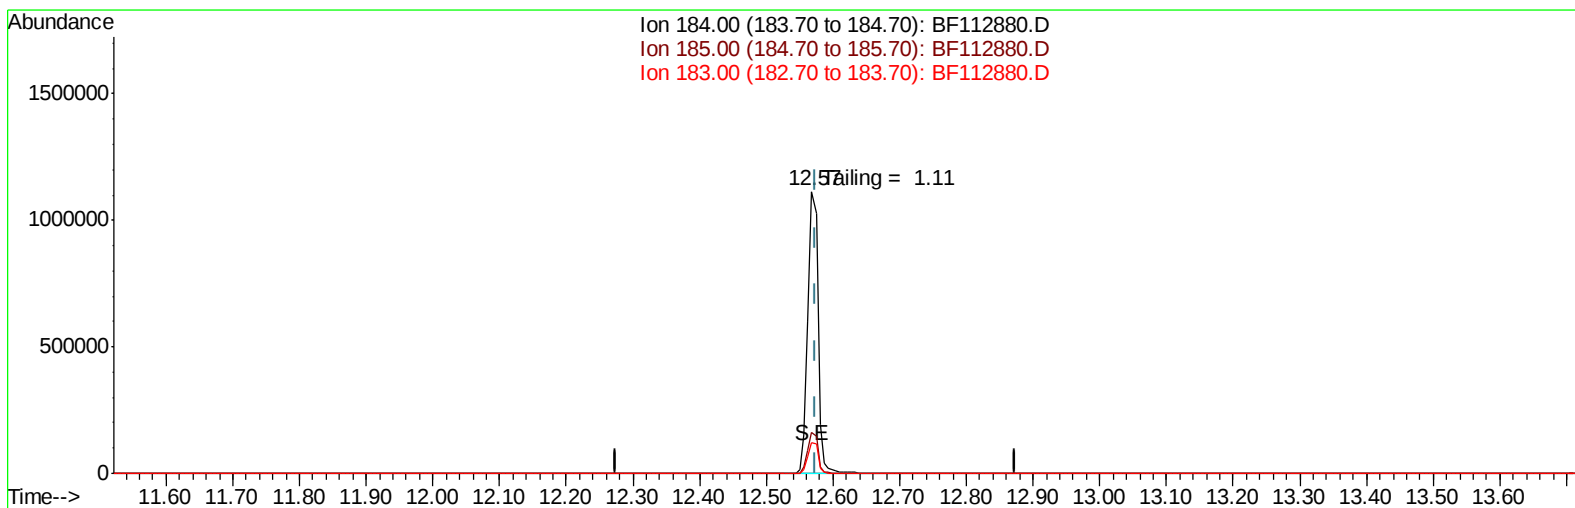

TIC: BF112880.D

(77) Benzidine

12.568min (-0.006) 7008.69ng

response 1138866

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.37 |
| 183.00 | 10.70 | 11.13 |
| 0.00   | 0.00  | 0.00  |