
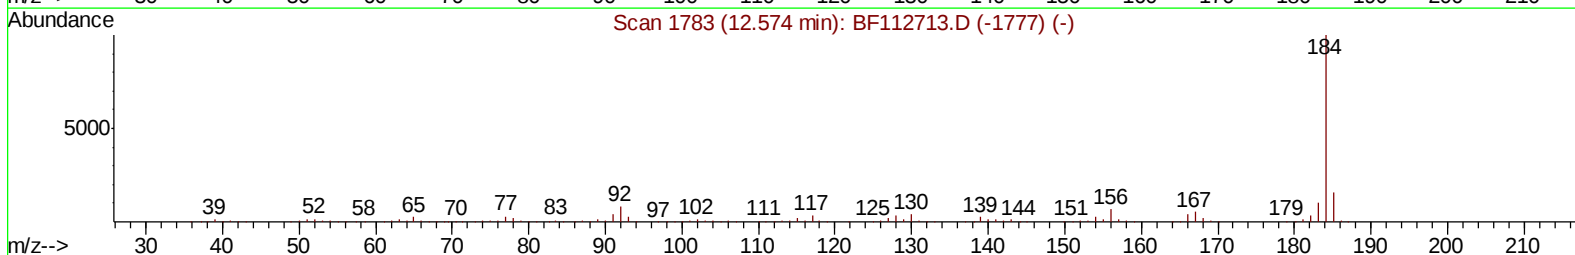
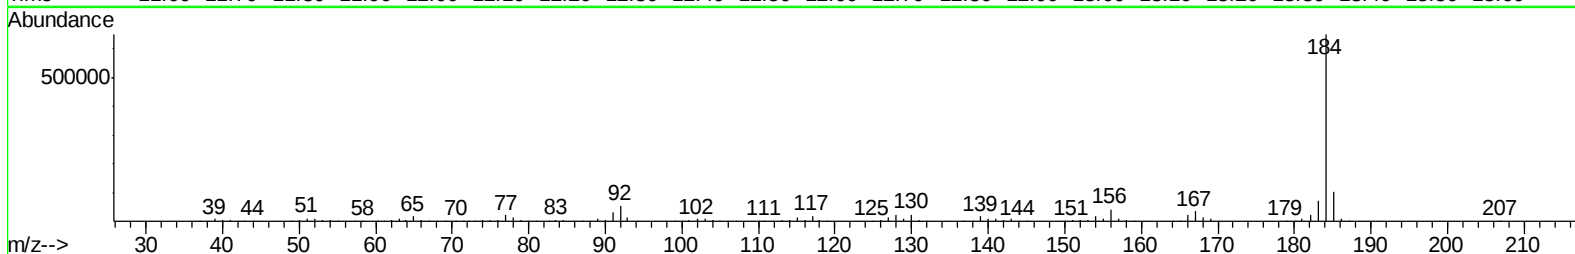


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030619\
 Data File : BF112898.D
 Acq On : 6 Mar 2019 23:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 06:00:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 01 15:40:43 2019
 Response via : Initial Calibration

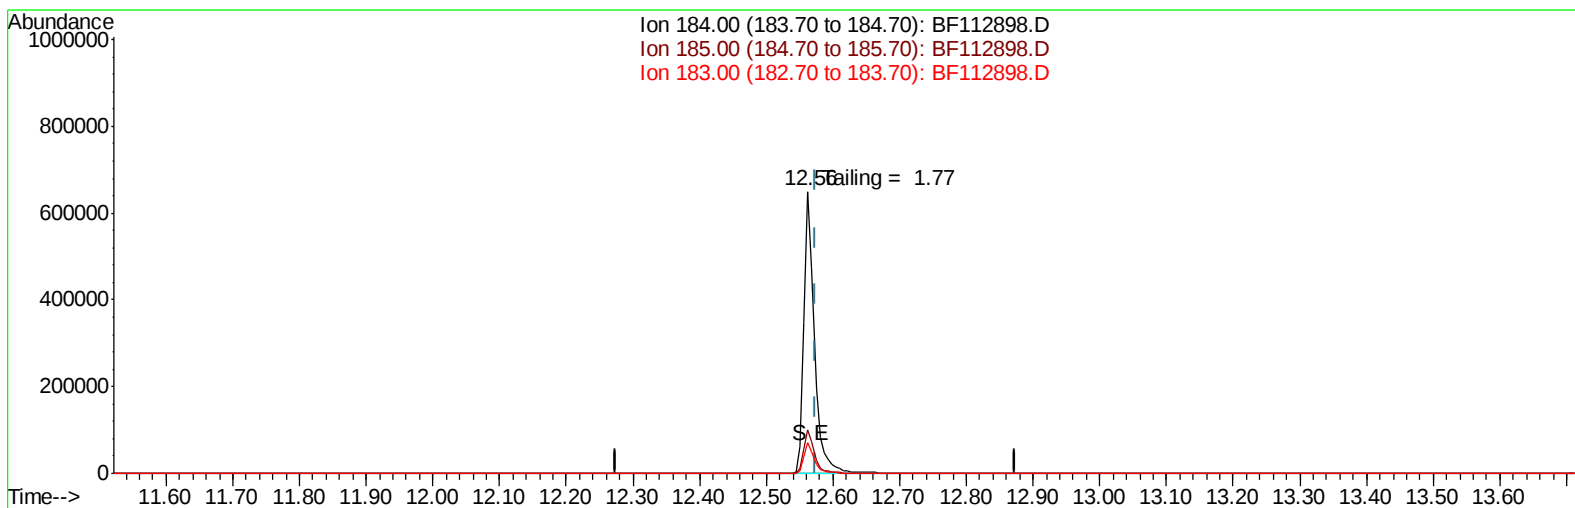

TIC: BF112898.D

(77) Benzidine




12.563min (-0.012) 11383.22ng

response 700429

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.52
183.00	10.70	10.87
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030619\
Data File : BF112898.D
Acq On : 6 Mar 2019 23:19
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 06:00:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 15:40:43 2019
Response via : Initial Calibration

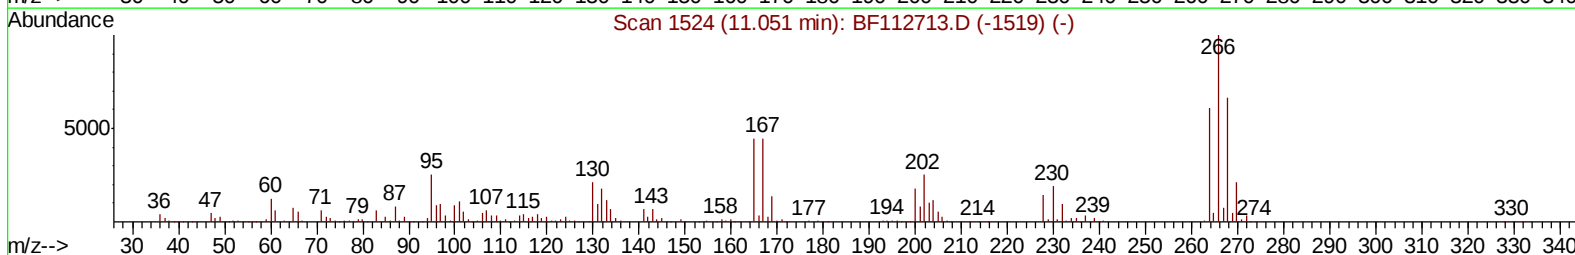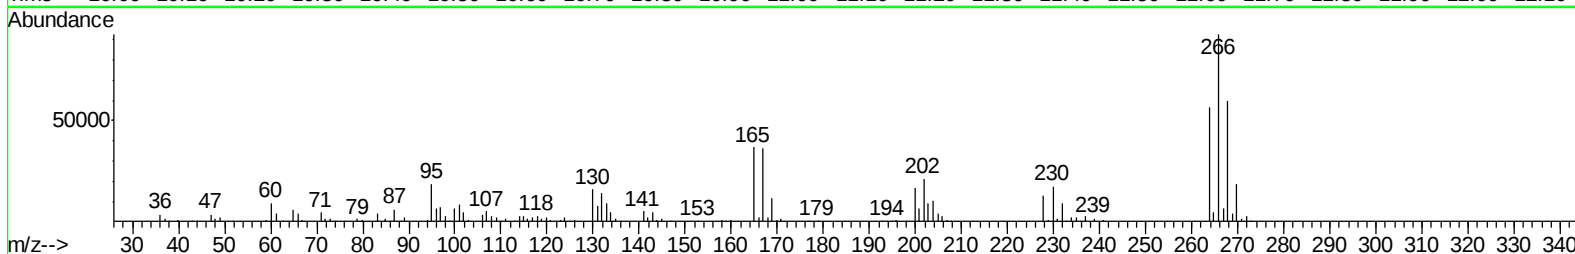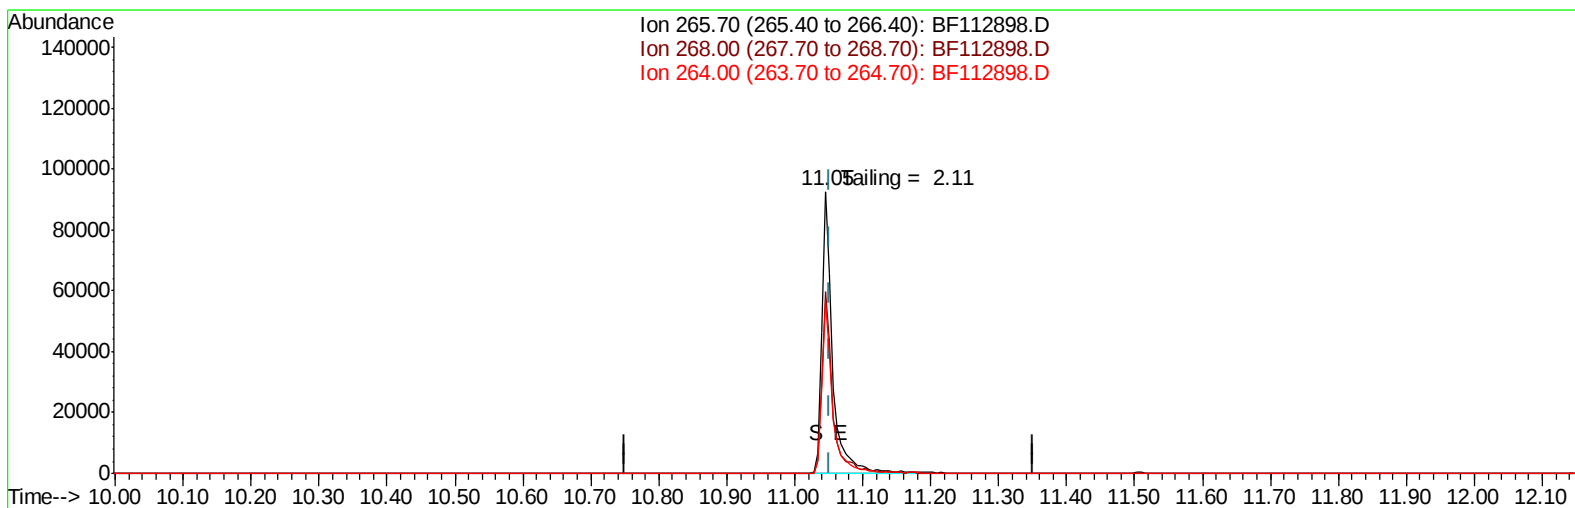

TIC: BF112898.D

(70) Pentachlorophenol (C)

11.045min (-0.006) 109599.82ng

response 103400

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.73
264.00	61.10	61.12
0.00	0.00	0.00