


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030619\
 Data File : BF112880.D
 Acq On : 6 Mar 2019 12:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 15:40:43 2019

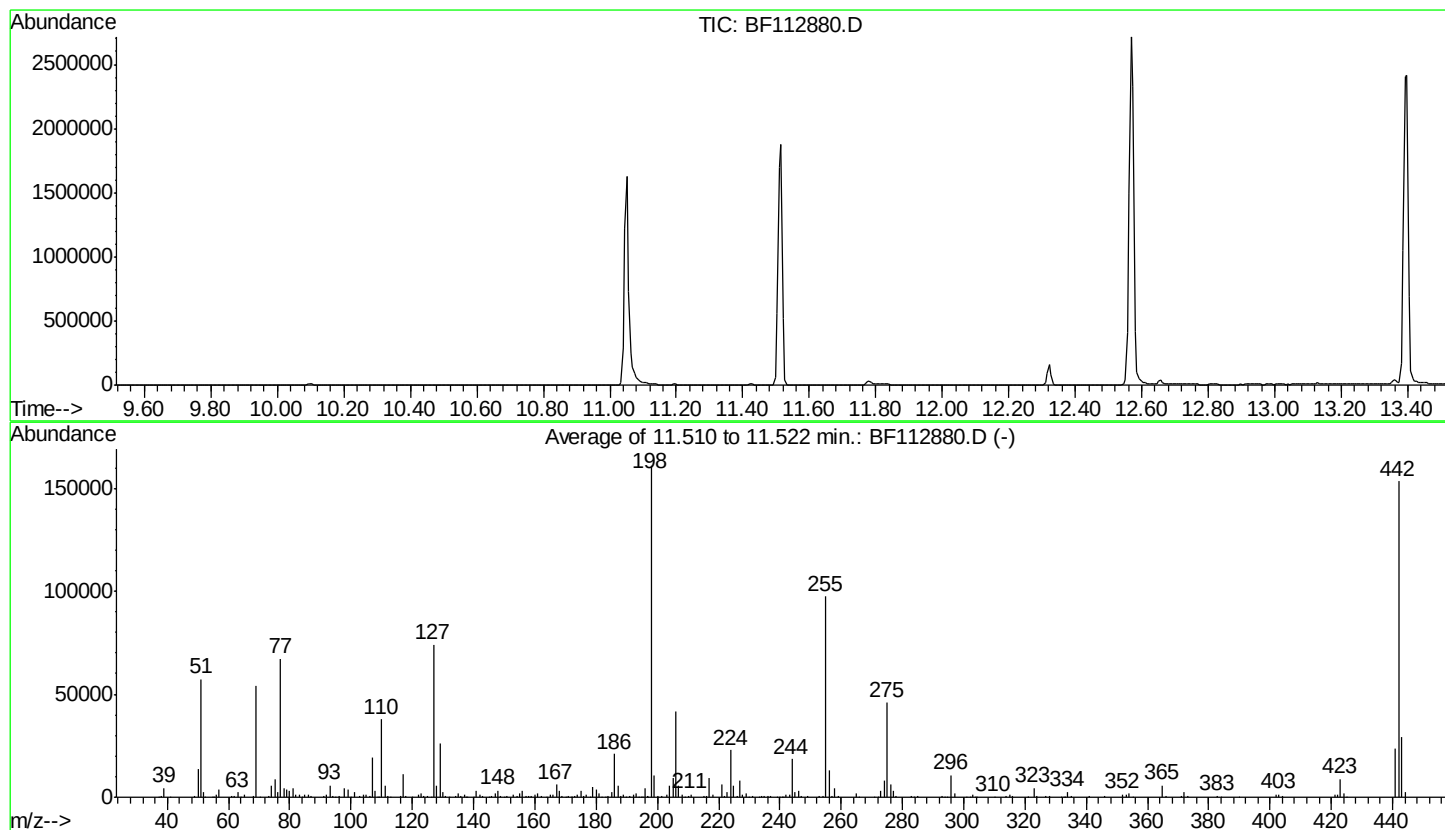

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	57479	PASS
68	69	0.00	2	1.5	799	PASS
69	198	0.00	100	33.7	54313	PASS
70	69	0.00	2	0.6	300	PASS
127	198	10	80	46.0	74130	PASS
197	198	0.00	2	0.5	734	PASS
198	198	100	100	100.0	160978	PASS
199	198	5	9	6.4	10372	PASS
275	198	10	60	28.4	45714	PASS
365	198	1	100	3.5	5633	PASS
441	198	0.01	100	14.8	23880	PASS
442	198	50	100	95.3	153376	PASS
443	442	15	24	18.9	29040	PASS