


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030619\
 Data File : BF112898.D
 Acq On : 6 Mar 2019 23:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 15:40:43 2019

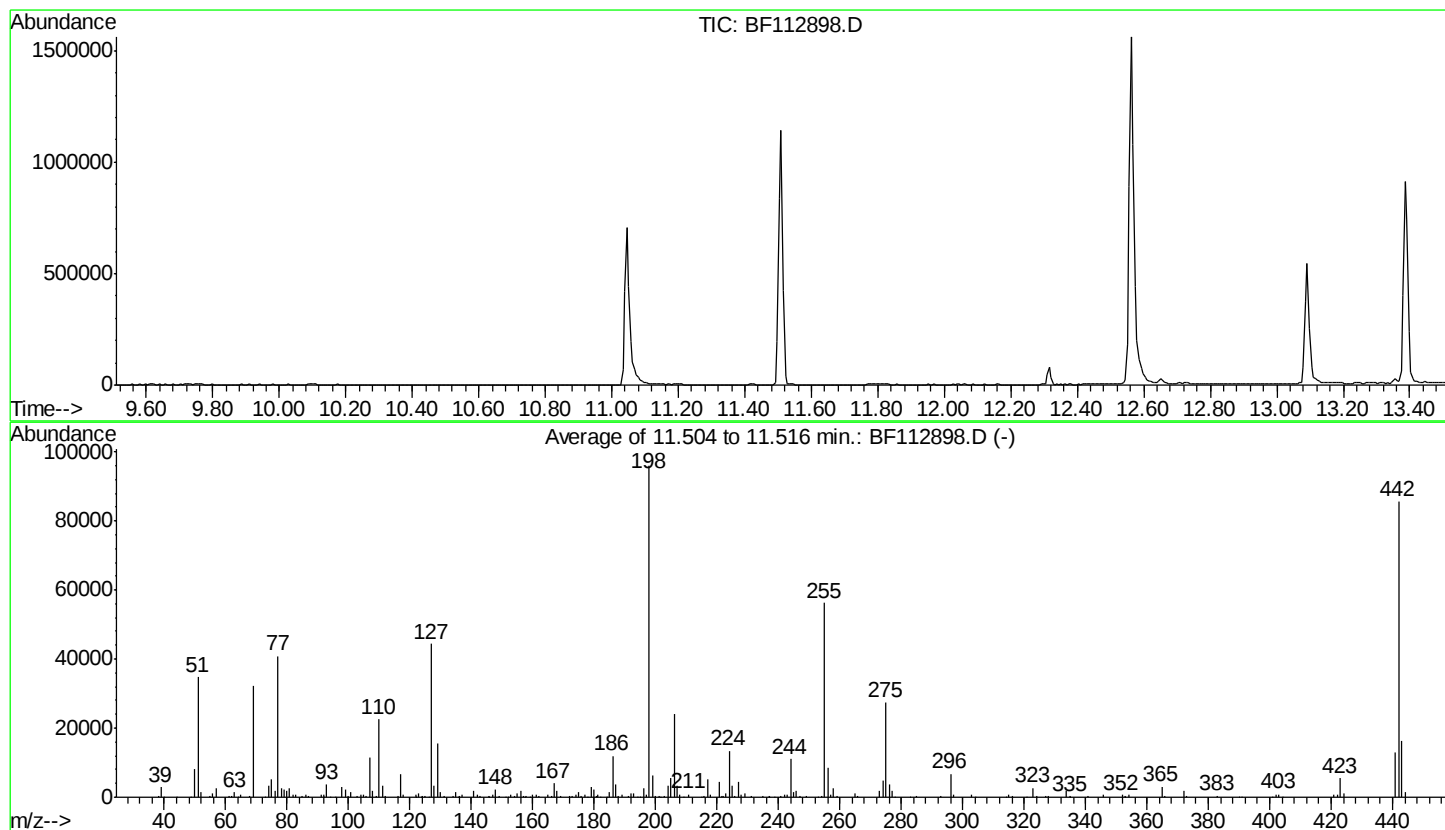

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	34663	PASS
68	69	0.00	2	1.6	515	PASS
69	198	0.00	100	33.7	32396	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.3	44432	PASS
197	198	0.00	2	0.6	582	PASS
198	198	100	100	100.0	95992	PASS
199	198	5	9	6.5	6211	PASS
275	198	10	60	28.5	27379	PASS
365	198	1	100	3.2	3082	PASS
441	198	0.01	100	13.7	13141	PASS
442	198	50	100	89.1	85557	PASS
443	442	15	24	19.1	16358	PASS