

Data File : BF119250.D

Acq On : 6 Mar 2020 14:39

Operator : CG/JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Mar 09 04:45:40 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Mar 06 23:38:46 2020

Response via : Initial Calibration

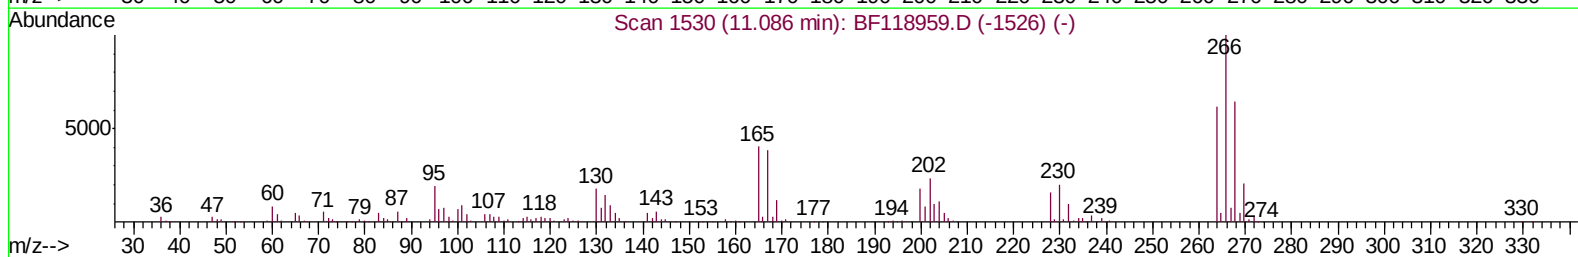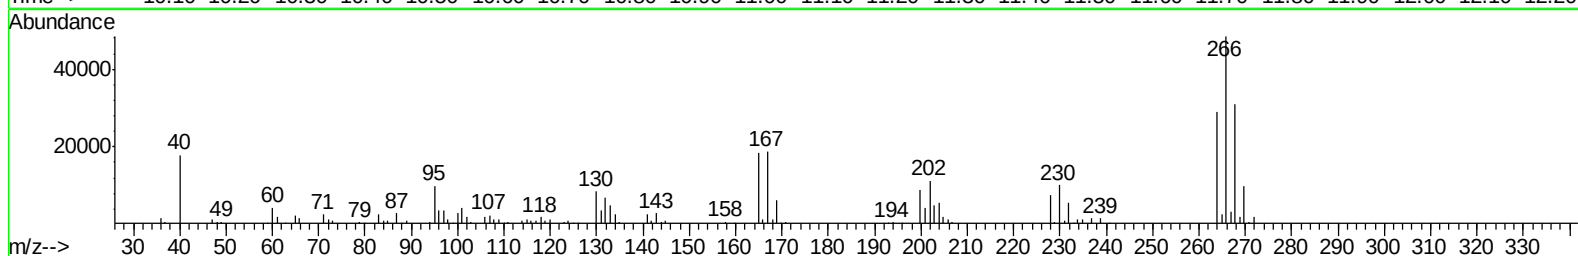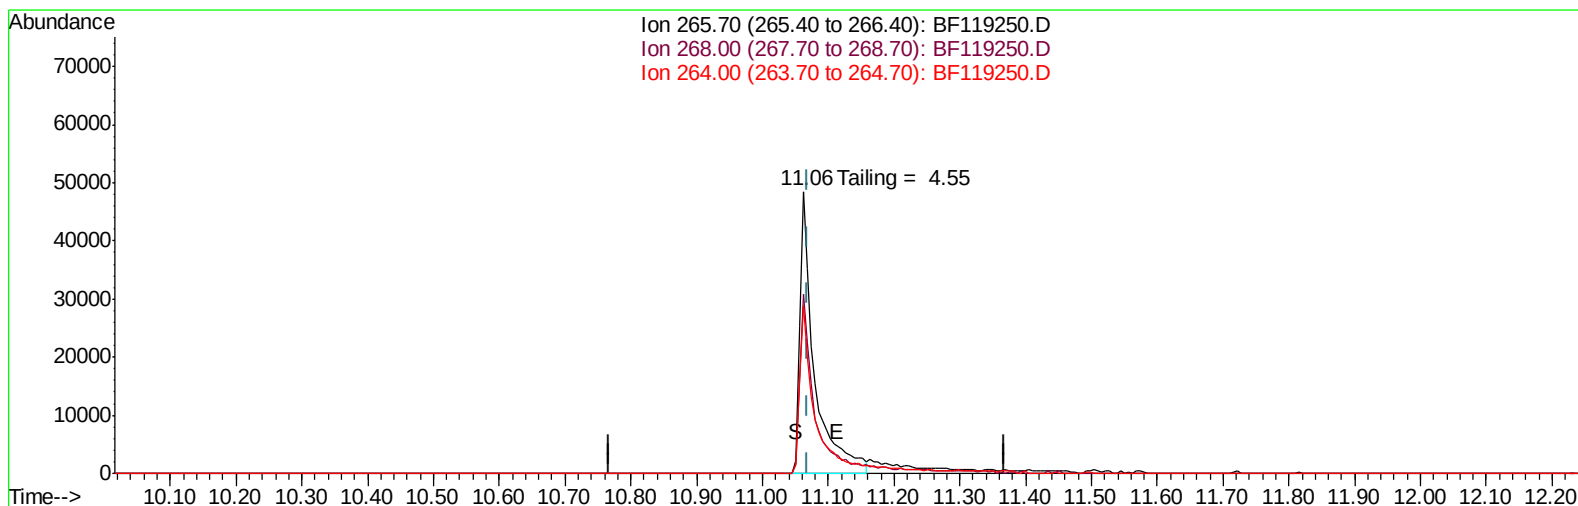

TIC: BF119250.D

(70) Pentachlorophenol (C)

11.063min (-0.006) 42107.74ng

response 82056

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	63.62
264.00	63.70	59.60
0.00	0.00	0.00

Data File : BF119250.D

Acq On : 6 Mar 2020 14:39

Operator : CG/JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Mar 09 04:45:40 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Mar 06 23:38:46 2020

Response via : Initial Calibration

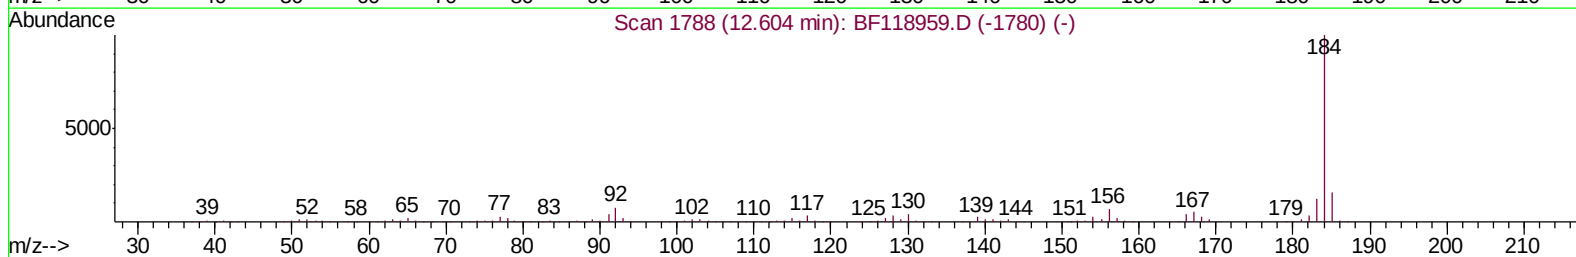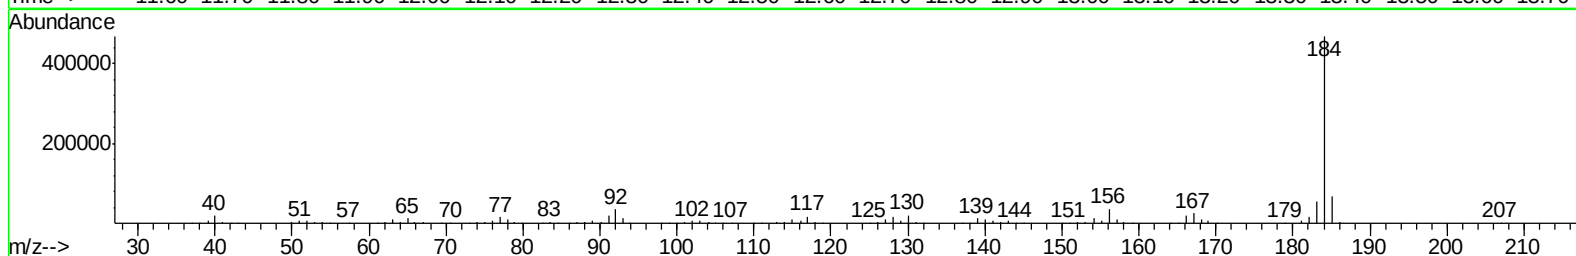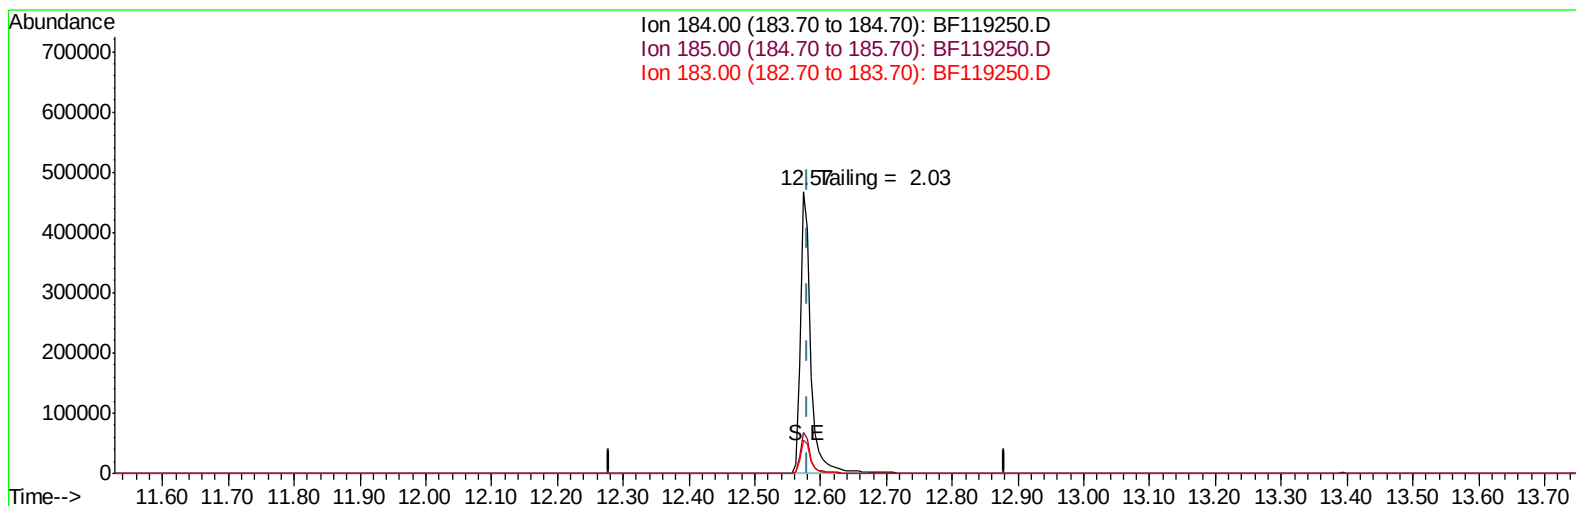

TIC: BF119250.D

(77) Benzidine

12.574min (-0.006) 0.00ng

response 513166

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.52
183.00	12.40	11.98
0.00	0.00	0.00