


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF030620\  
 Data File : BF119250.D  
 Acq On : 6 Mar 2020 14:39  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF022020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 06 23:38:46 2020

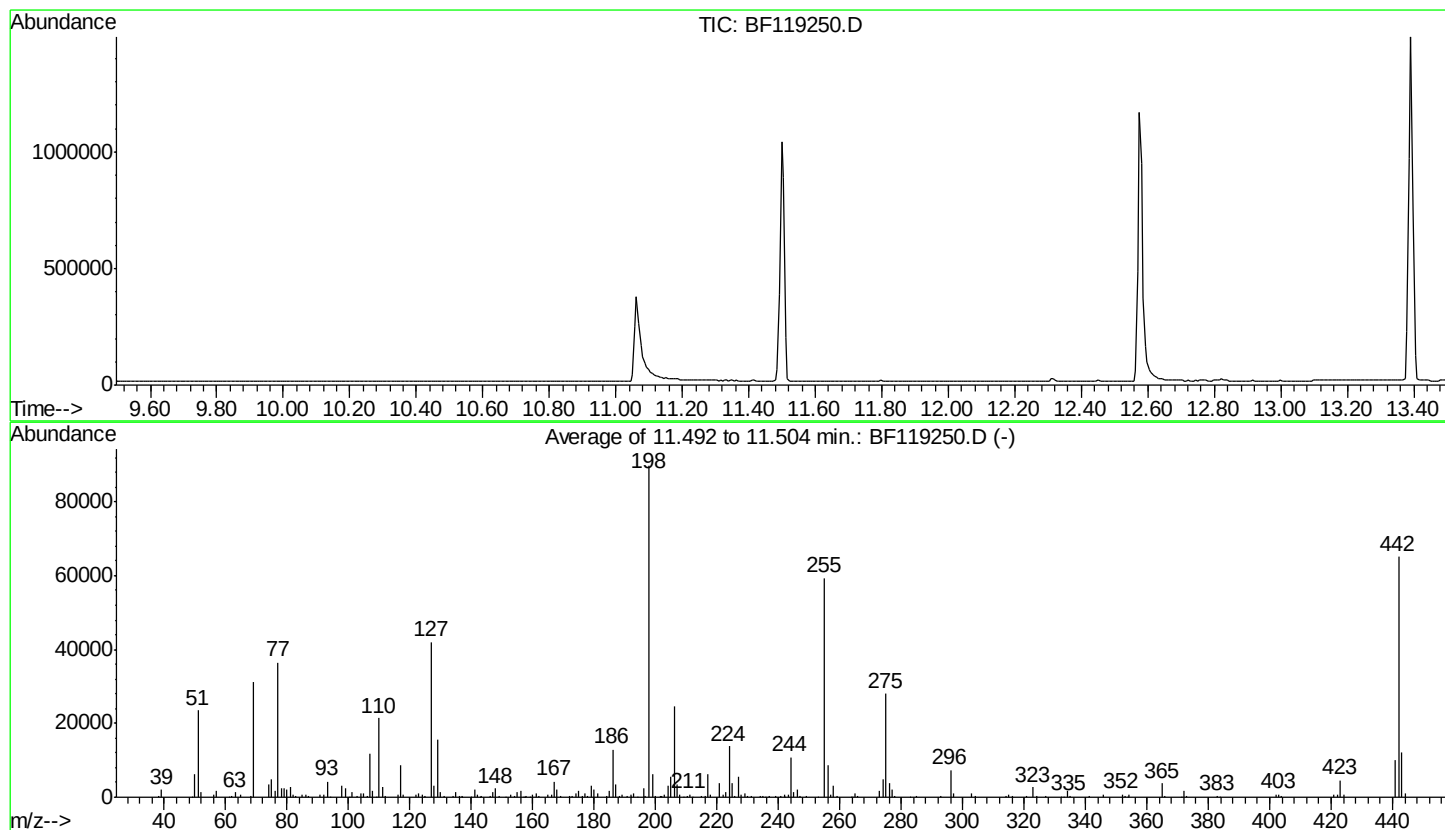

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 26.2      | 23490   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.6       | 201     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.8      | 31288   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 46.7      | 41962   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 349     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 89794   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 6090    | PASS             |
| 275         | 198          | 10           | 60           | 31.2      | 28019   | PASS             |
| 365         | 198          | 1            | 100          | 4.2       | 3735    | PASS             |
| 441         | 198          | 0.01         | 100          | 11.3      | 10180   | PASS             |
| 442         | 198          | 50           | 100          | 72.5      | 65103   | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 12212   | PASS             |