


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030620\
 Data File : BF119274.D
 Acq On : 7 Mar 2020 3:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 06 23:38:46 2020

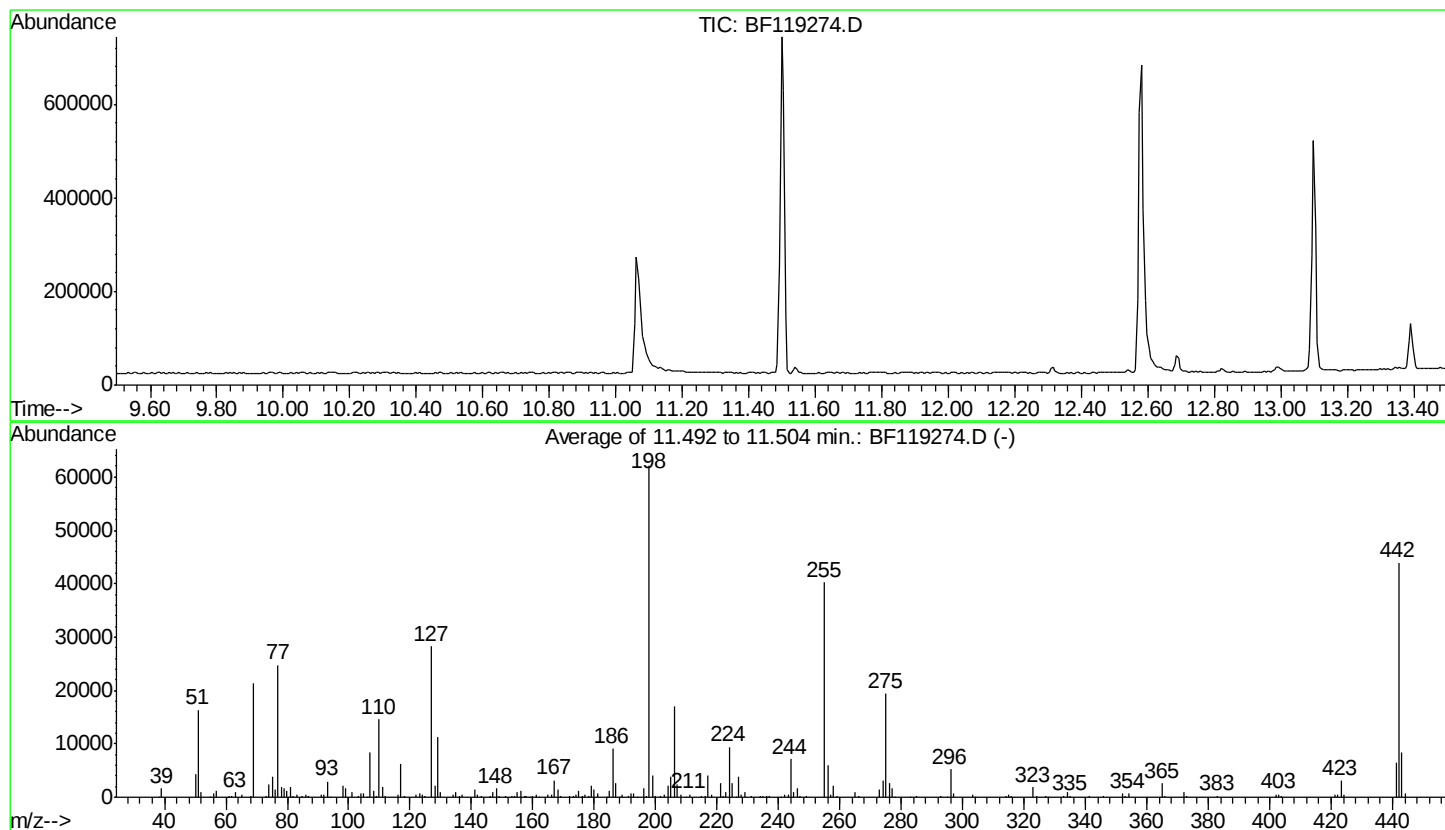

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	16376	PASS
68	69	0.00	2	1.4	297	PASS
69	198	0.00	100	34.5	21431	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.5	28283	PASS
197	198	0.00	2	0.4	234	PASS
198	198	100	100	100.0	62122	PASS
199	198	5	9	6.7	4156	PASS
275	198	10	60	31.2	19386	PASS
365	198	1	100	4.2	2596	PASS
441	198	0.01	100	10.6	6587	PASS
442	198	50	100	70.7	43903	PASS
443	442	15	24	18.9	8309	PASS