


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030819\
 Data File : BF112936.D
 Acq On : 8 Mar 2019 11:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 15:40:43 2019

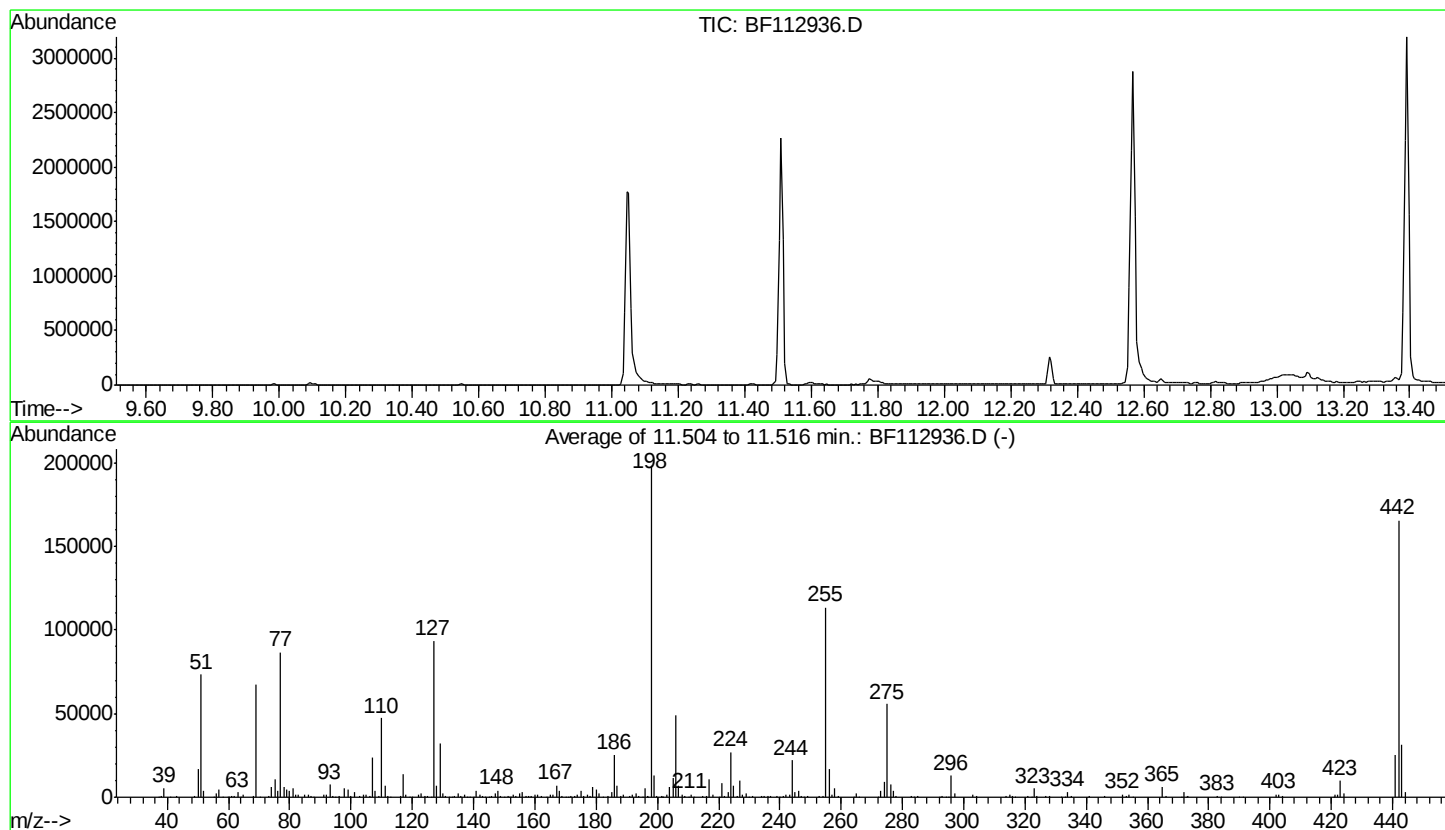

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	73269	PASS
68	69	0.00	2	1.6	1043	PASS
69	198	0.00	100	33.9	67122	PASS
70	69	0.00	2	0.4	301	PASS
127	198	10	80	47.2	93578	PASS
197	198	0.00	2	0.5	926	PASS
198	198	100	100	100.0	198186	PASS
199	198	5	9	6.7	13283	PASS
275	198	10	60	28.0	55530	PASS
365	198	1	100	3.1	6235	PASS
441	198	0.01	100	12.6	25048	PASS
442	198	50	100	83.5	165394	PASS
443	442	15	24	19.2	31716	PASS