
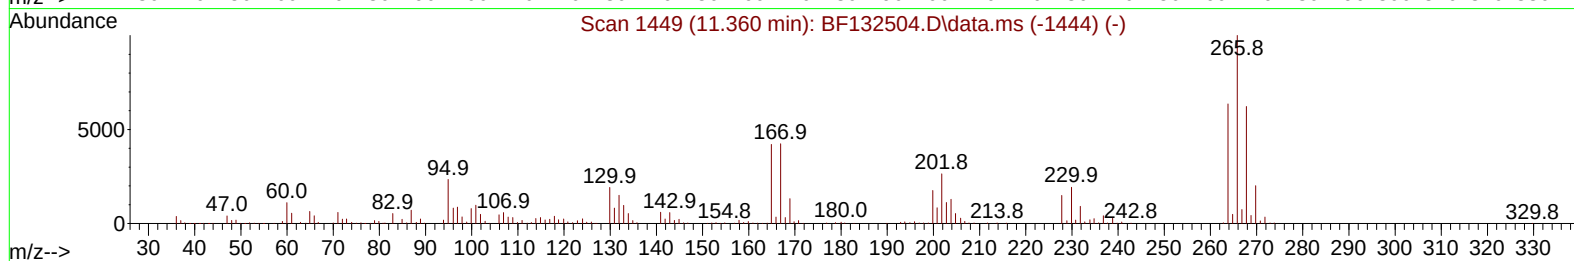
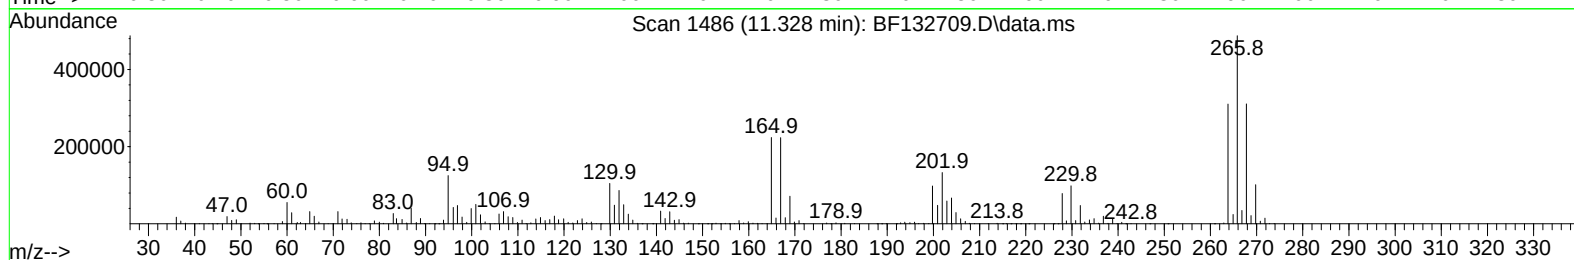


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132709.D
Acq On : 09 Mar 2023 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 04:27:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 16:26:19 2023
Response via : Initial Calibration

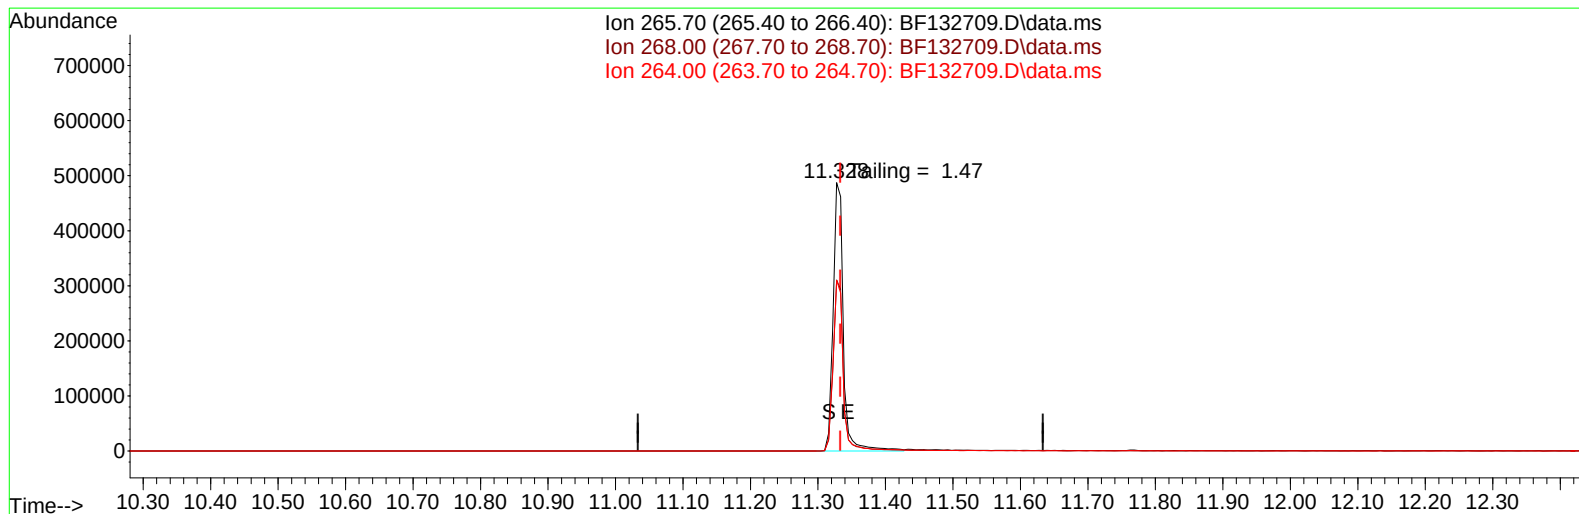

TIC: BF132709.D\data.ms

(70) Pentachlorophenol (C)




11.328min (-0.006) 274062.60 ng

response 510424

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.73
264.00	63.60	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
 Data File : BF132709.D
 Acq On : 09 Mar 2023 10:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 04:27:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 16:26:19 2023
 Response via : Initial Calibration

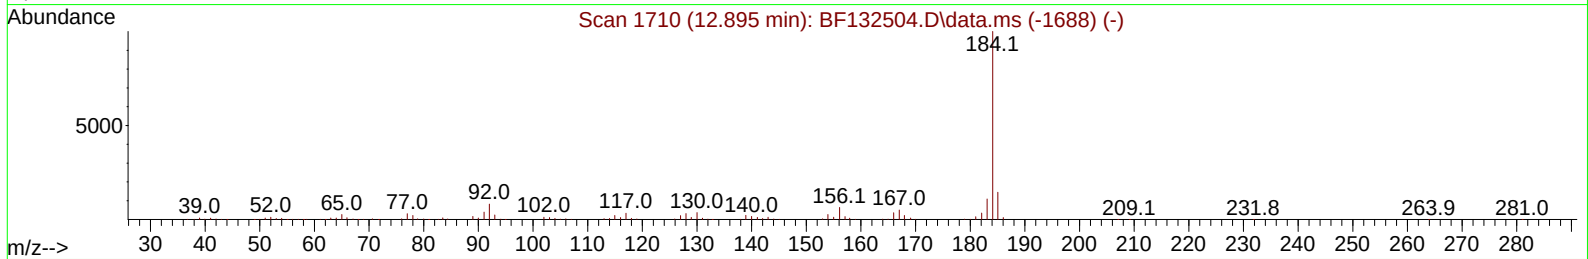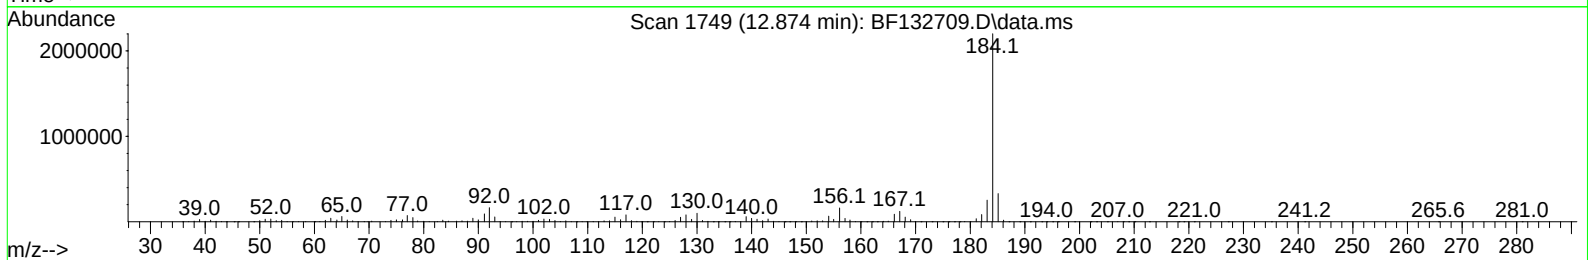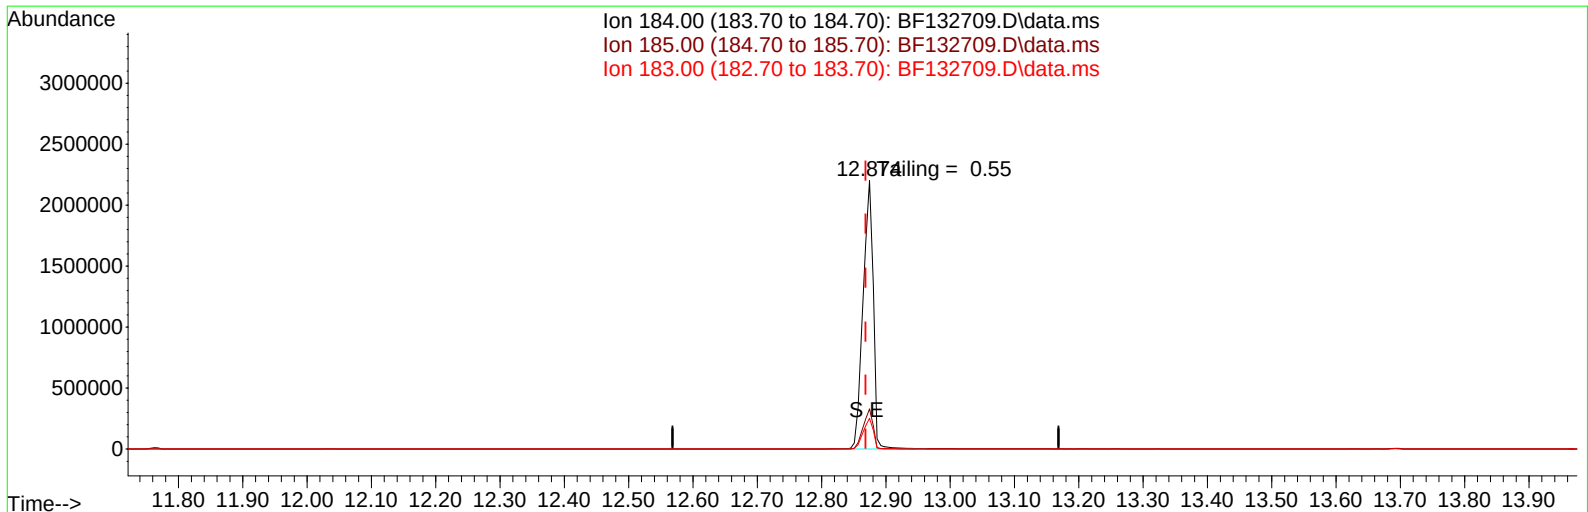

TIC: BF132709.D\data.ms

(77) Benzidine

12.874min (+ 0.006) 26133.89 ng

response 2427638

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	15.01
183.00	10.90	11.48
0.00	0.00	0.00