

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
 Data File : BF132711.D
 Acq On : 09 Mar 2023 11:15
 Operator : CG\JU
 Sample : PB151294TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB151294TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	444	450	464	rBV	2147409	3147636	36.63%	5.907%
2	5.628	512	517	520	rBV	5872353	6340619	73.78%	11.899%
3	6.622	680	686	689	rBV	5442816	6293004	73.22%	11.810%
4	6.981	743	747	750	rBV	1840377	1487311	17.31%	2.791%
5	7.551	838	844	847	rBV	4288058	4393338	51.12%	8.245%
6	8.263	961	965	969	rBV	2172136	1914721	22.28%	3.593%
7	9.345	1142	1149	1152	rBV	8184551	7697486	89.57%	14.446%
8	10.027	1261	1265	1268	rBV	2752658	2269055	26.40%	4.258%
9	10.827	1396	1401	1404	rBV	5342014	5343739	62.18%	10.029%
10	11.521	1515	1519	1523	rBV	2755634	2496441	29.05%	4.685%
11	13.121	1785	1791	1794	rBV	8841515	8594139	100.00%	16.129%
12	14.186	1967	1972	1975	rBV	1943176	1887582	21.96%	3.542%
13	15.727	2229	2234	2242	rVB	1053634	1419753	16.52%	2.664%




Sum of corrected areas: 53284824

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132711.D
Acq On : 09 Mar 2023 11:15
Operator : CG\JU
Sample : PB151294TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151294TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

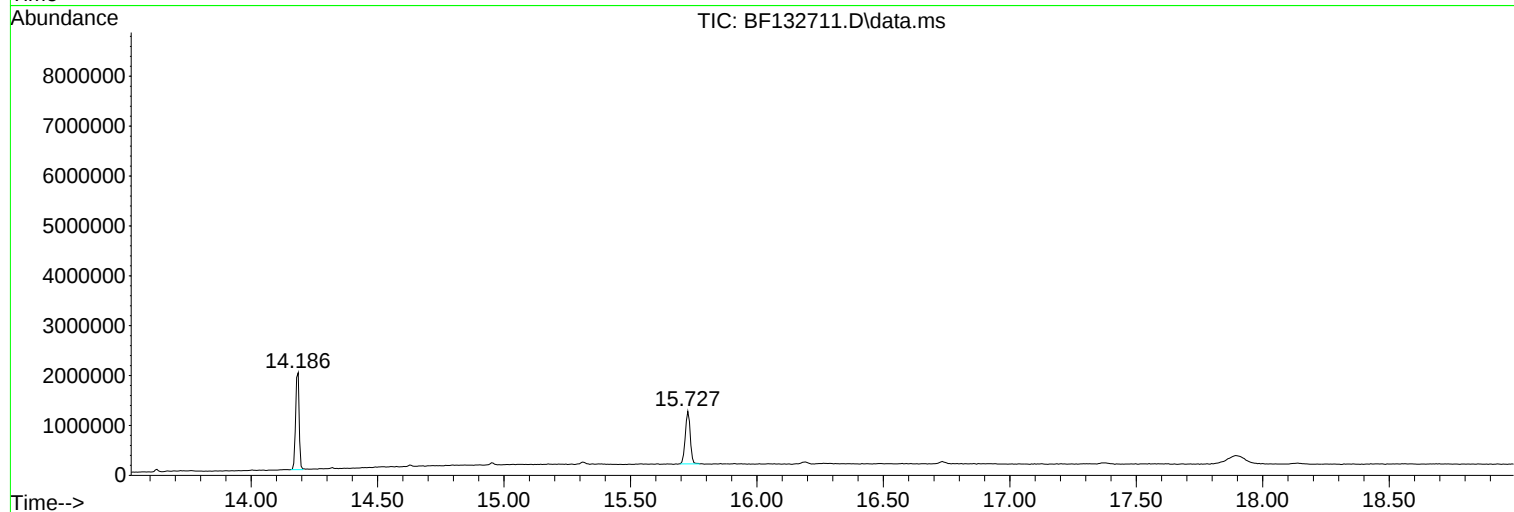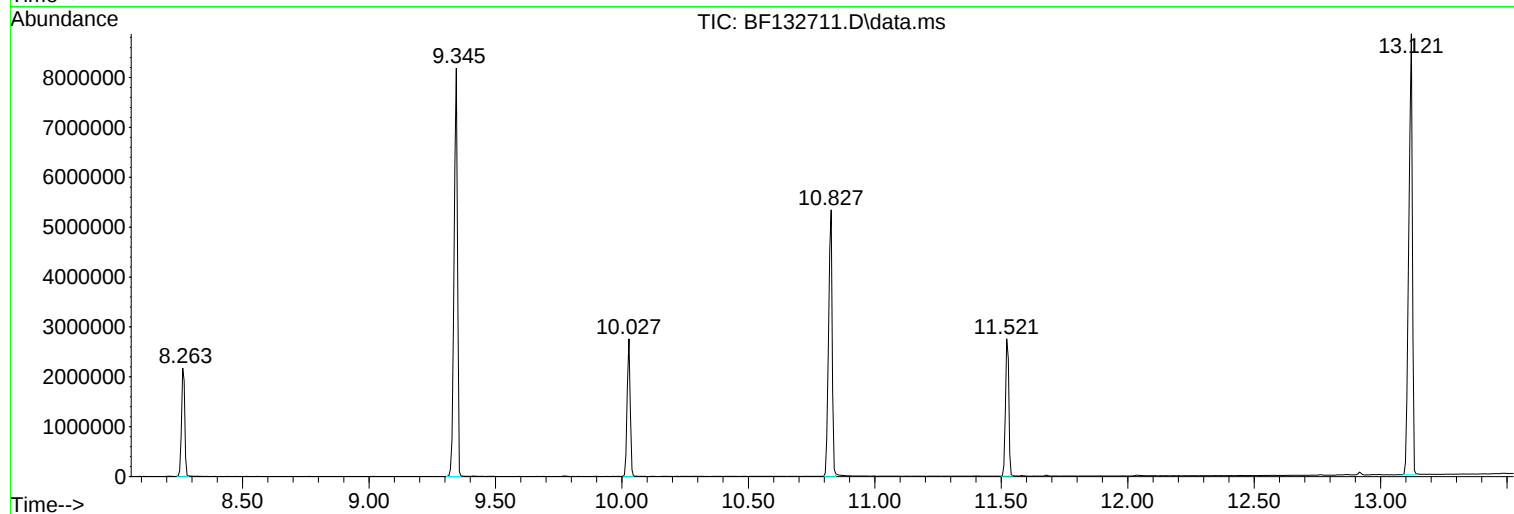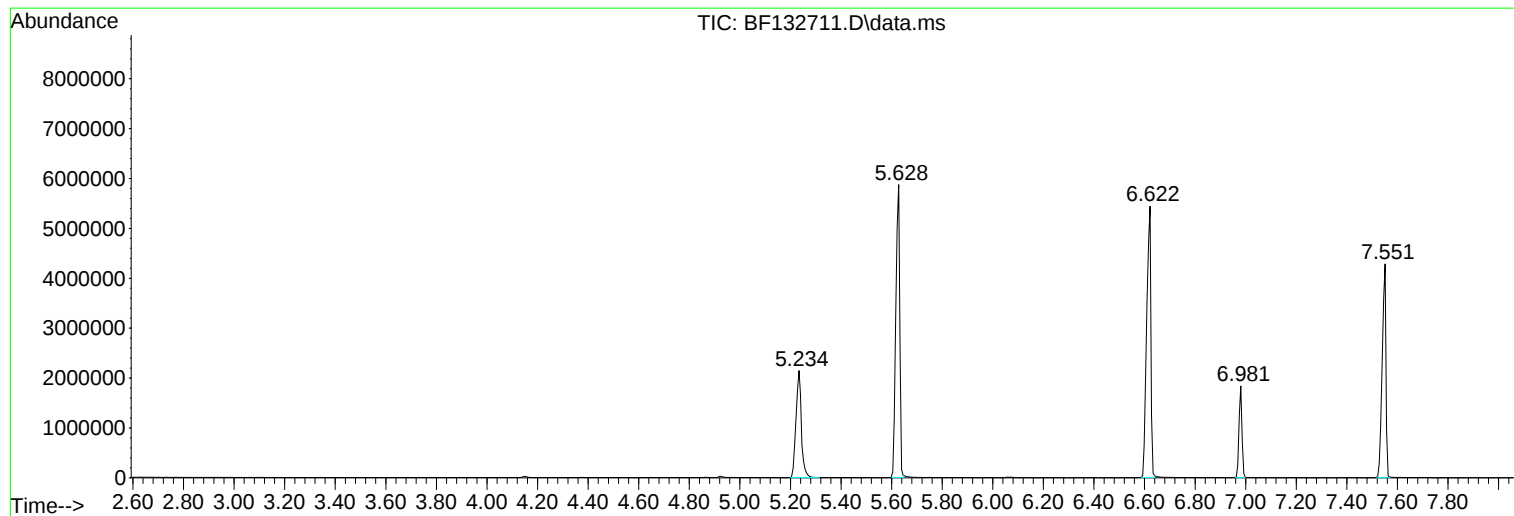

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132711.D
Acq On : 09 Mar 2023 11:15
Operator : CG\JU
Sample : PB151294TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151294TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132711.D
Acq On : 09 Mar 2023 11:15
Operator : CG\JU
Sample : PB151294TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB151294TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------