

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
 Data File : BF132717.D
 Acq On : 09 Mar 2023 14:37
 Operator : CG\JU
 Sample : 01833-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 11

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.075	77	83	92	rVB	357330	521519	9.14%	1.364%
2	3.910	216	225	232	rVB	58951	83750	1.47%	0.219%
3	4.128	259	262	270	rVB	125138	158651	2.78%	0.415%
4	4.263	280	285	291	rBV	87282	103049	1.81%	0.270%
5	4.616	339	345	352	rVB2	88556	114381	2.00%	0.299%
6	4.804	373	377	383	rVV	183768	174581	3.06%	0.457%
7	4.869	383	388	394	rVB	125598	135868	2.38%	0.355%
8	5.228	444	449	463	rVB	2284814	3009027	52.74%	7.870%
9	5.622	512	516	526	rBV	4756387	4574833	80.18%	11.965%
10	6.616	680	685	688	rBV	4152411	4116372	72.15%	10.766%
11	6.804	713	717	724	rBV	65679	70453	1.23%	0.184%
12	6.981	743	747	750	rBV	1283185	1084873	19.01%	2.837%
13	7.545	838	843	846	rBV	3452530	3315952	58.12%	8.673%
14	7.640	855	859	868	rVB2	119884	146063	2.56%	0.382%
15	8.263	961	965	969	rBV	1679296	1363704	23.90%	3.567%
16	9.339	1144	1148	1151	rBV	6434136	5705563	100.00%	14.923%
17	10.022	1261	1264	1268	rBV	1679931	1502918	26.34%	3.931%
18	10.822	1395	1400	1403	rBV	3575968	3276962	57.43%	8.571%
19	11.522	1515	1519	1522	rBV	1568210	1305129	22.87%	3.414%
20	13.110	1785	1789	1793	rBV	4806702	4762369	83.47%	12.456%
21	14.180	1967	1971	1974	rBV	1275180	1130125	19.81%	2.956%
22	14.269	1981	1986	1991	rBV	460972	503217	8.82%	1.316%
23	15.721	2228	2233	2242	rVB	826544	1074682	18.84%	2.811%




Sum of corrected areas: 38234041

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132717.D
Acq On : 09 Mar 2023 14:37
Operator : CG\JU
Sample : 01833-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

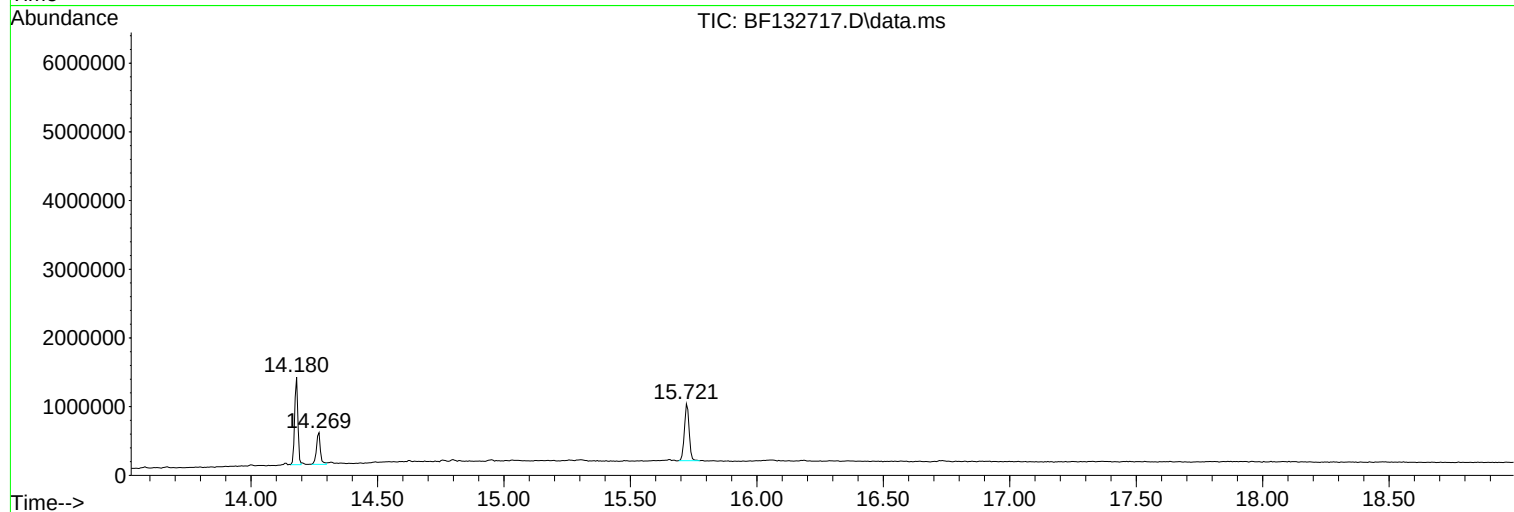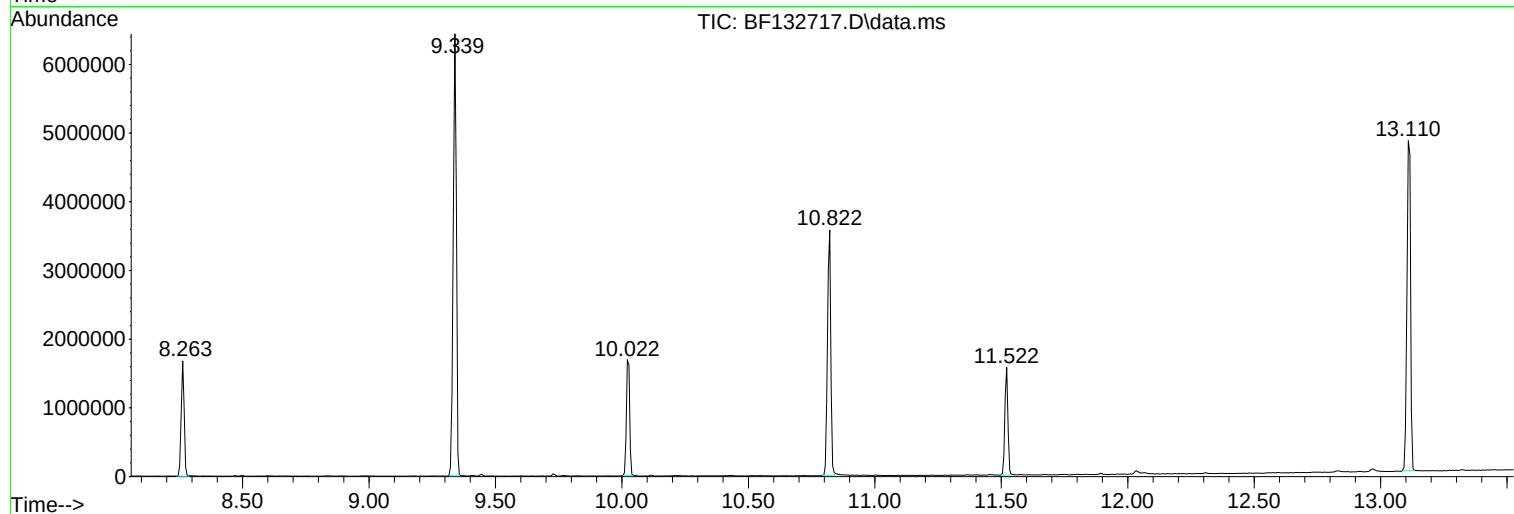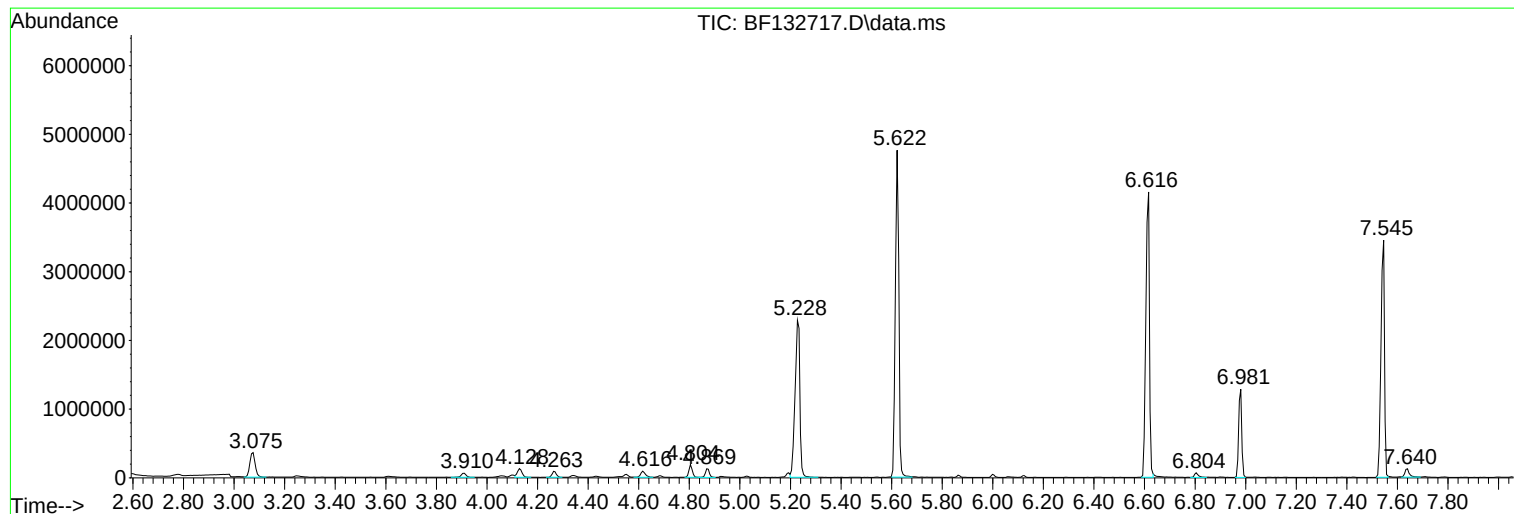

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132717.D
Acq On : 09 Mar 2023 14:37
Operator : CG\JU
Sample : 01833-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132717.D
Acq On : 09 Mar 2023 14:37
Operator : CG\JU
Sample : 01833-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------