

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
 Data File : BF132722.D
 Acq On : 09 Mar 2023 17:23
 Operator : CG\JU
 Sample : 01833-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 46

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.087	80	85	96	rVB	295690	419944	7.33%	1.036%
2	3.916	221	226	233	rVB	49651	69189	1.21%	0.171%
3	4.134	260	263	271	rVB	139361	176587	3.08%	0.436%
4	4.269	281	286	291	rBV	71856	82686	1.44%	0.204%
5	4.628	341	347	354	rBV	750563	836023	14.59%	2.063%
6	4.810	370	378	384	rVV	131733	163279	2.85%	0.403%
7	4.875	384	389	396	rVB2	109162	117412	2.05%	0.290%
8	5.193	439	443	444	rBV	71472	64922	1.13%	0.160%
9	5.228	444	449	460	rVB	1993734	2472116	43.14%	6.099%
10	5.622	512	516	519	rBV	4831116	4643367	81.03%	11.456%
11	6.281	625	628	636	rBV	50772	70571	1.23%	0.174%
12	6.616	680	685	697	rBV	4300276	4448194	77.62%	10.975%
13	6.804	714	717	727	rVB	106239	114957	2.01%	0.284%
14	6.981	743	747	750	rBV	1374964	1143789	19.96%	2.822%
15	7.545	838	843	846	rBV	3635628	3336052	58.22%	8.231%
16	8.263	961	965	968	rBV	1973027	1506191	26.28%	3.716%
17	9.339	1144	1148	1151	rBV	6704973	5730482	100.00%	14.138%
18	10.022	1261	1264	1268	rVB	1795011	1563438	27.28%	3.857%
19	10.822	1395	1400	1403	rBV	3686425	3441533	60.06%	8.491%
20	11.522	1515	1519	1522	rBV	1543273	1418526	24.75%	3.500%
21	12.033	1603	1606	1618	rBV2	451008	529703	9.24%	1.307%
22	12.822	1737	1740	1754	rBV	315094	405378	7.07%	1.000%
23	13.110	1785	1789	1792	rBV	5216577	4875683	85.08%	12.029%
24	14.180	1967	1971	1975	rBV	1308664	1198902	20.92%	2.958%
25	14.263	1981	1985	1992	rBV	492264	514163	8.97%	1.269%
26	15.721	2228	2233	2242	rVB	898842	1188825	20.75%	2.933%




Sum of corrected areas: 40531912

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132722.D
Acq On : 09 Mar 2023 17:23
Operator : CG\JU
Sample : 01833-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
46

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

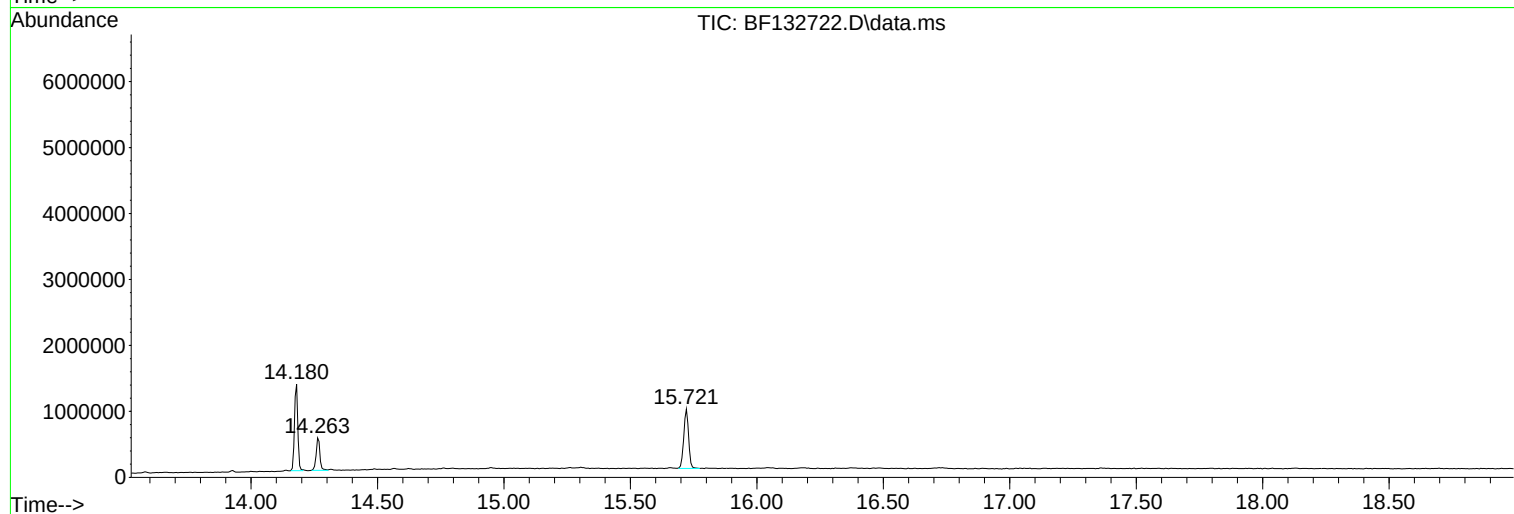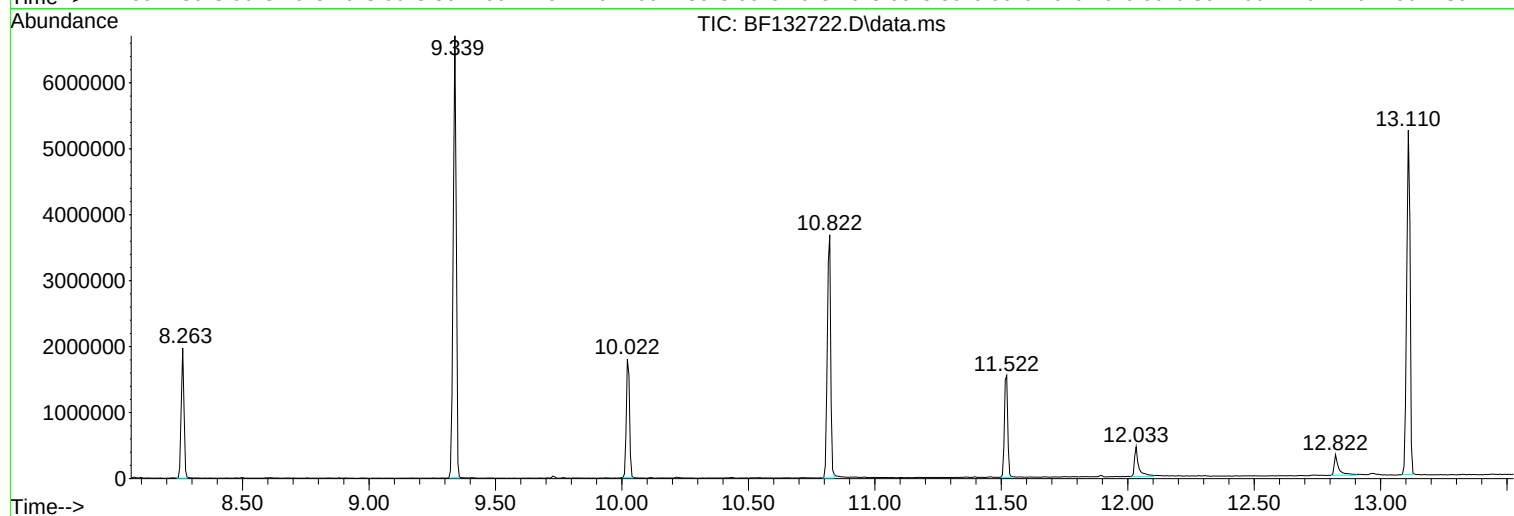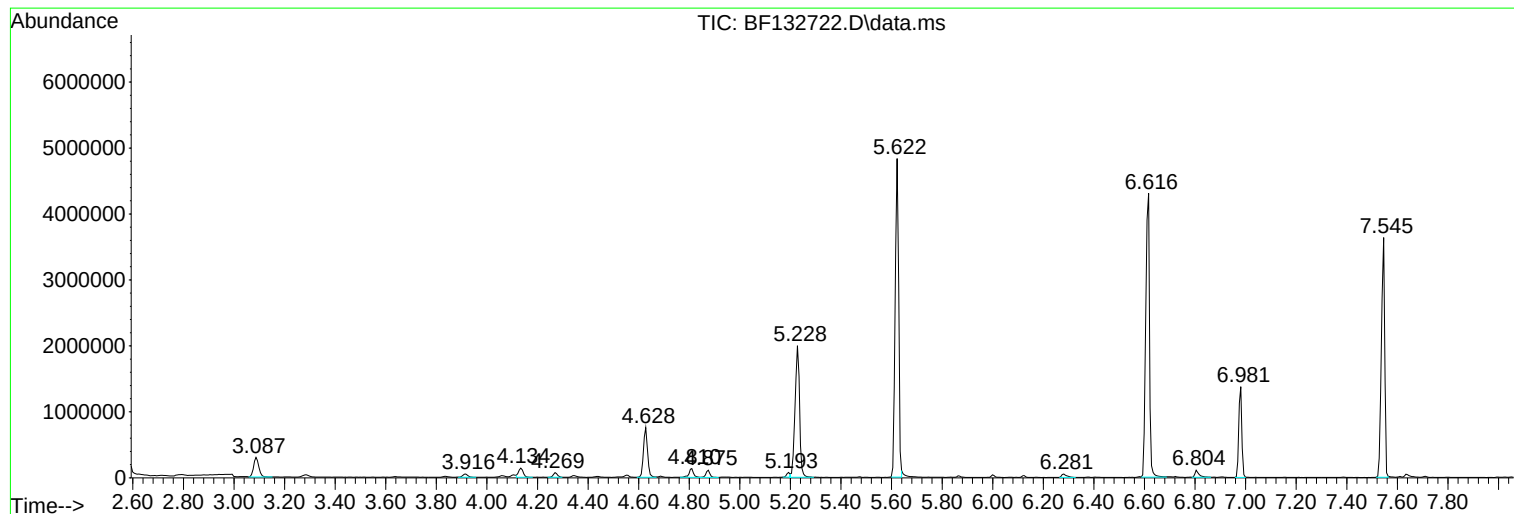

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132722.D
Acq On : 09 Mar 2023 17:23
Operator : CG\JU
Sample : 01833-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
46

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132722.D
Acq On : 09 Mar 2023 17:23
Operator : CG\JU
Sample : 01833-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
46

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------