


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
Data File : BF132709.D
Acq On : 09 Mar 2023 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 09 16:26:19 2023

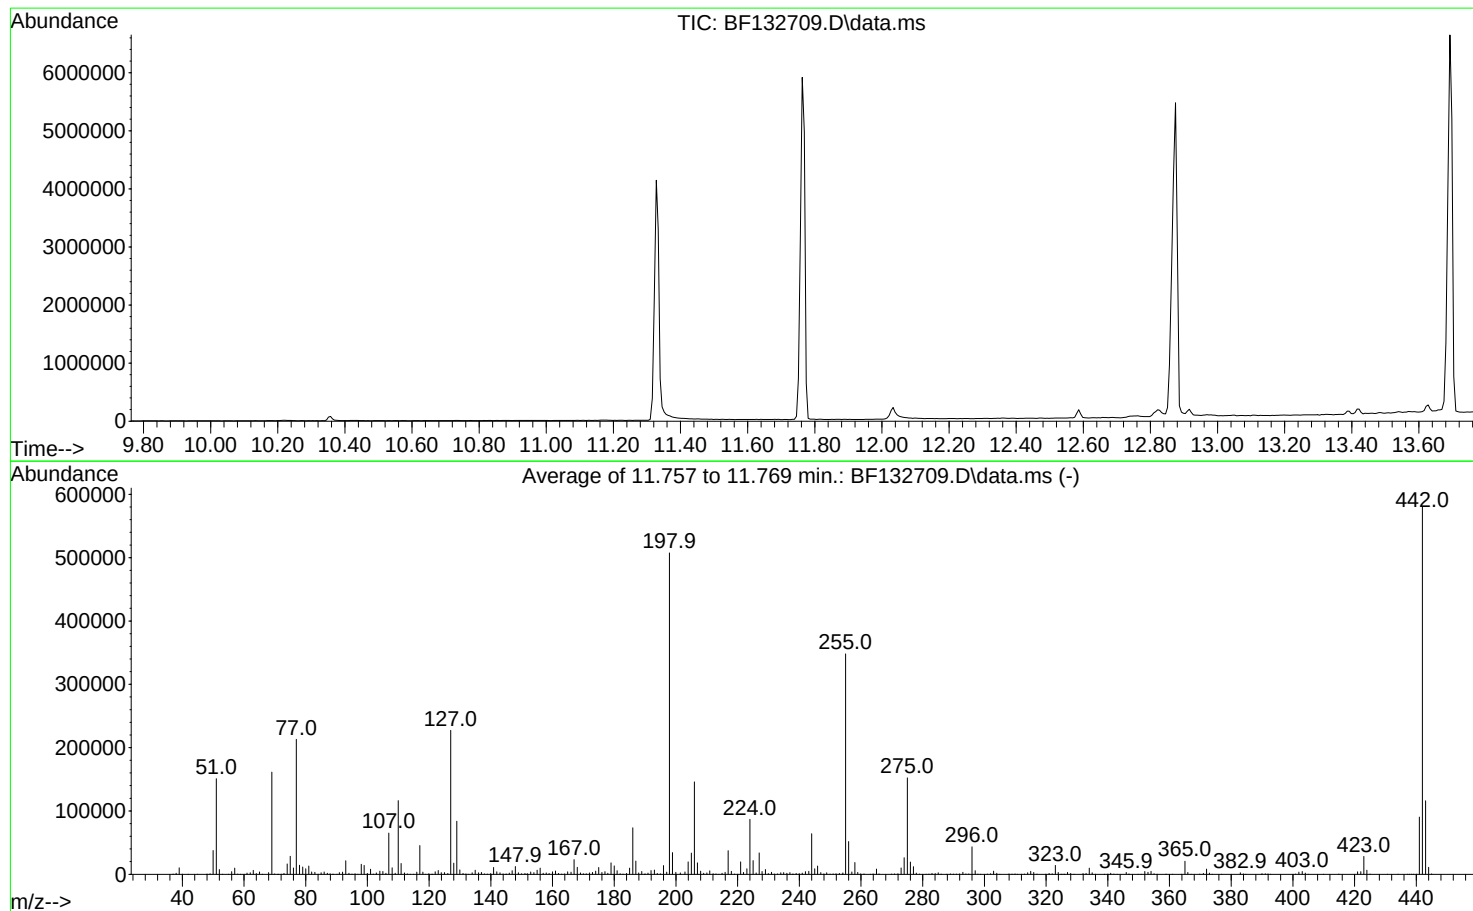




AutoFind: Scans 1559, 1560, 1561; Background Corrected with Scan 1553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	150891	PASS
68	69	0.00	2	1.7	2706	PASS
69	198	0.00	100	31.8	161433	PASS
70	69	0.00	2	0.4	591	PASS
127	198	10	80	44.8	227328	PASS
197	198	0.00	2	0.7	3526	PASS
198	198	100	100	100.0	507669	PASS
199	198	5	9	6.8	34277	PASS
275	198	10	60	30.0	152317	PASS
365	198	1	100	4.1	20708	PASS
441	198	0.01	100	17.8	90248	PASS
442	442	50	100	100.0	580949	PASS
443	442	15	24	20.0	116027	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
 Data File : BF132709.D
 Acq On : 09 Mar 2023 10:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 10 04:27:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 16:26:19 2023
 Response via : Initial Calibration

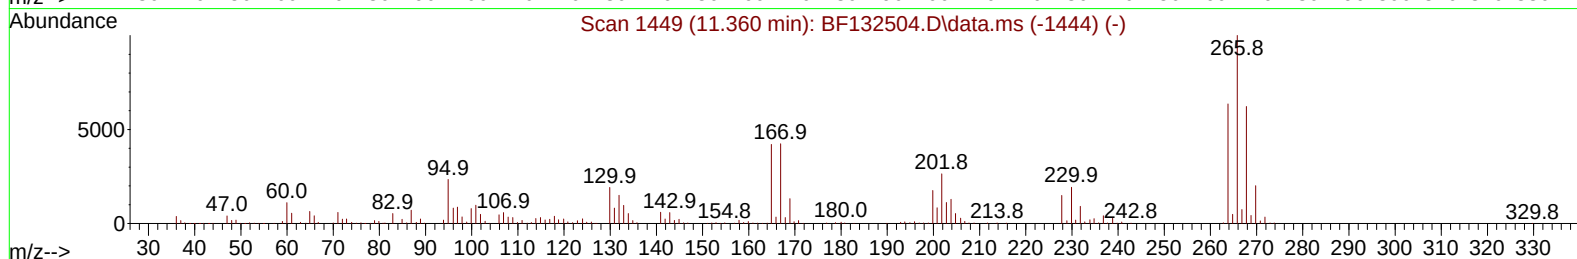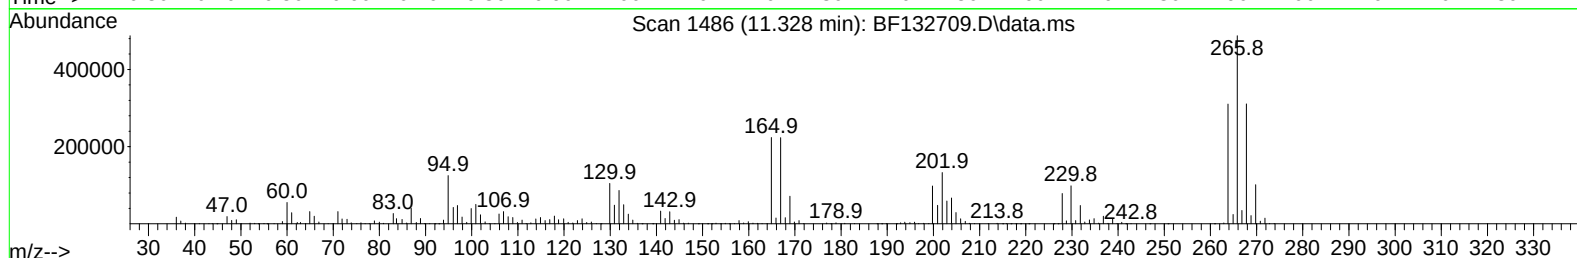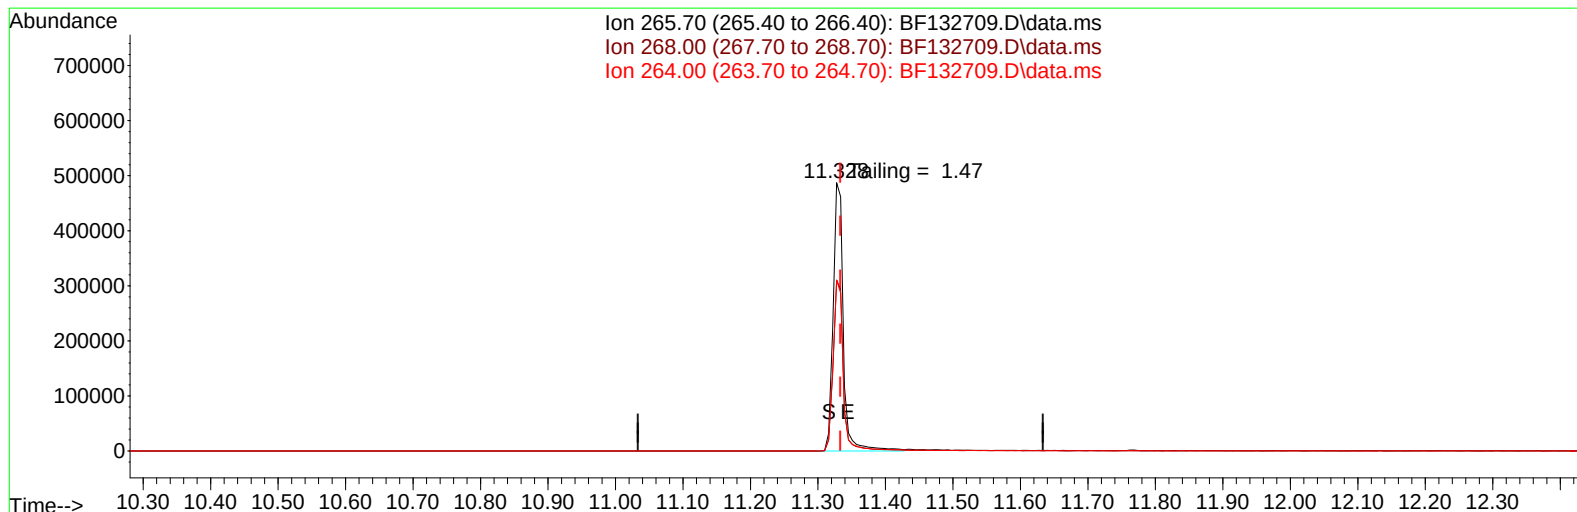

TIC: BF132709.D\data.ms

(70) Pentachlorophenol (C)

11.328min (-0.006) 274062.60 ng




response 510424

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.73
264.00	63.60	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030923\
 Data File : BF132709.D
 Acq On : 09 Mar 2023 10:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 10 04:27:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 16:26:19 2023
 Response via : Initial Calibration

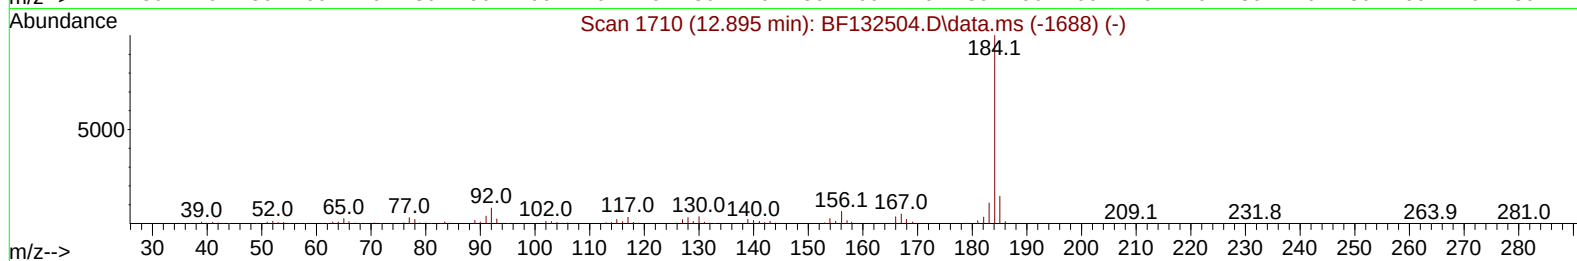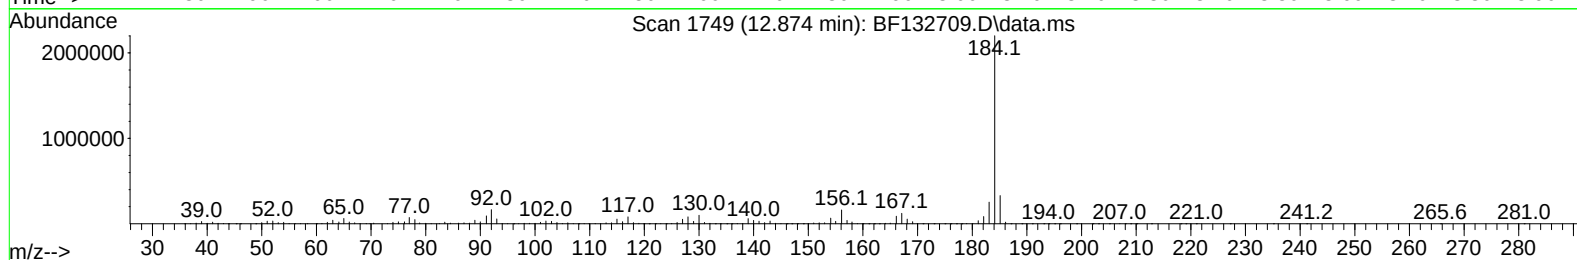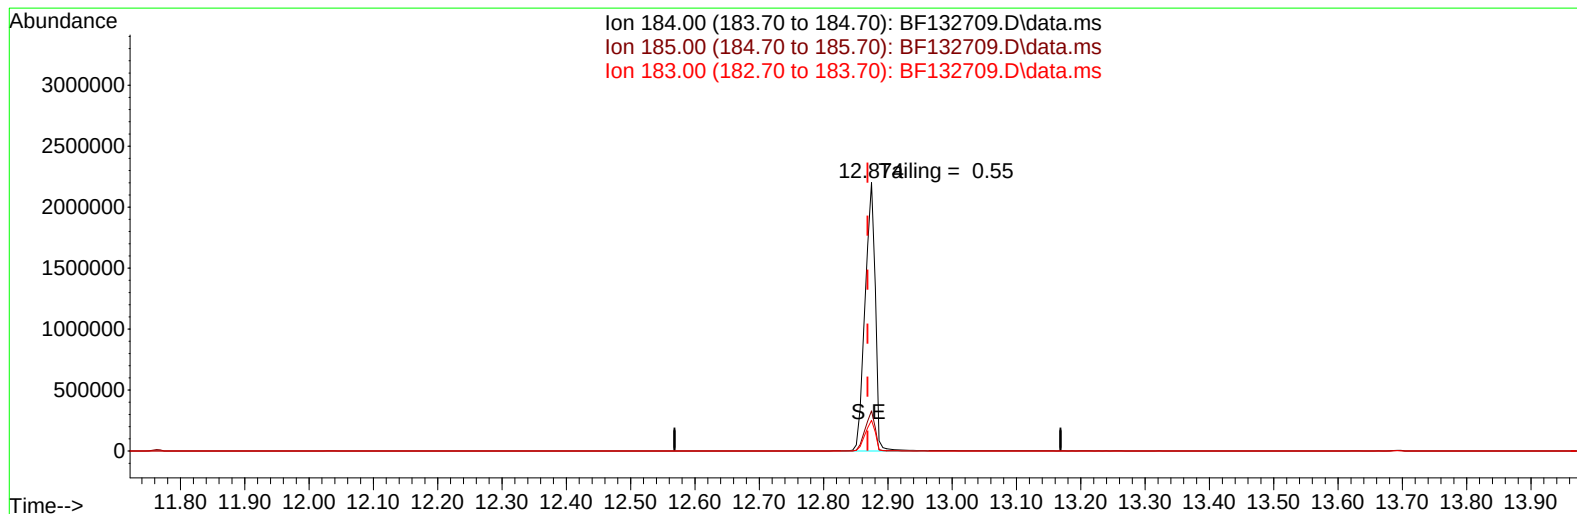

TIC: BF132709.D\data.ms

(77) Benzidine

12.874min (+ 0.006) 26133.89 ng

response 2427638

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	15.01
183.00	10.90	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/9/2023	BNA_F	<u>BF132709.D</u>
Compound Name	Response	Retention Time
DDT	1282951	13.629
DDD	29087	13.422
DDE	1501	13.057
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30588	1313539	2.33

Instrument :
BNA_F
ClientSampleId :
DFTPP