
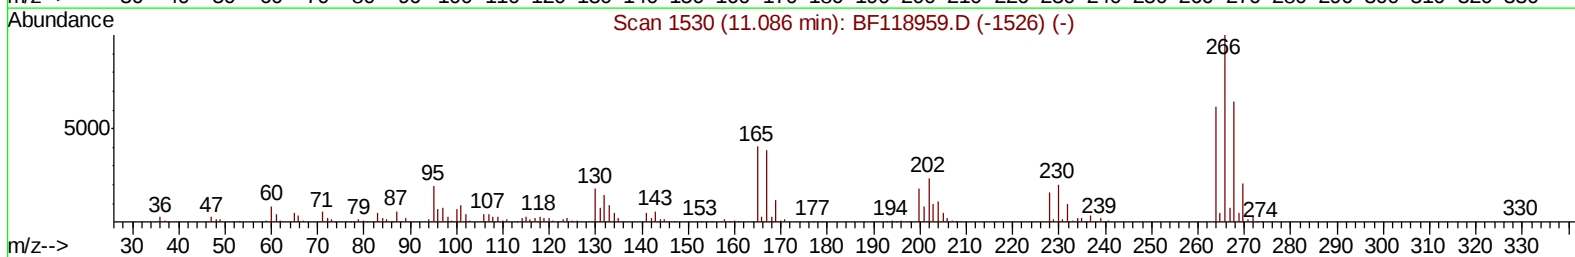
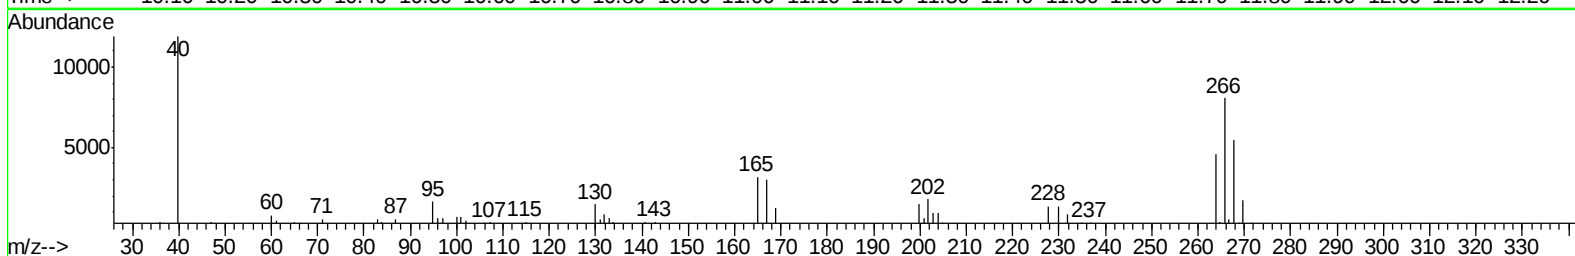


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF031020\
Data File : BF119330.D
Acq On : 10 Mar 2020 23:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 07:12:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

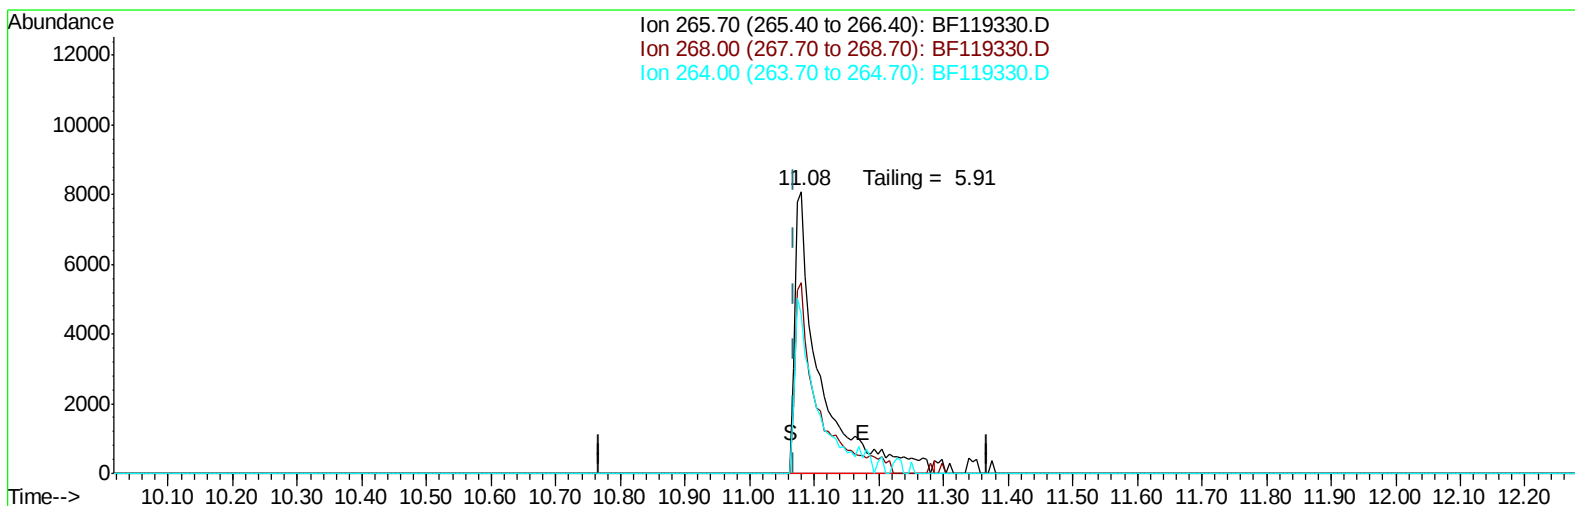

TIC: BF119330.D

(70) Pentachlorophenol (C)




11.080min (+0.012) 28391.81ng m

response 21545

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	67.78
264.00	63.70	56.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF031020\
 Data File : BF119330.D
 Acq On : 10 Mar 2020 23:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 07:12:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 06 23:38:46 2020
 Response via : Initial Calibration

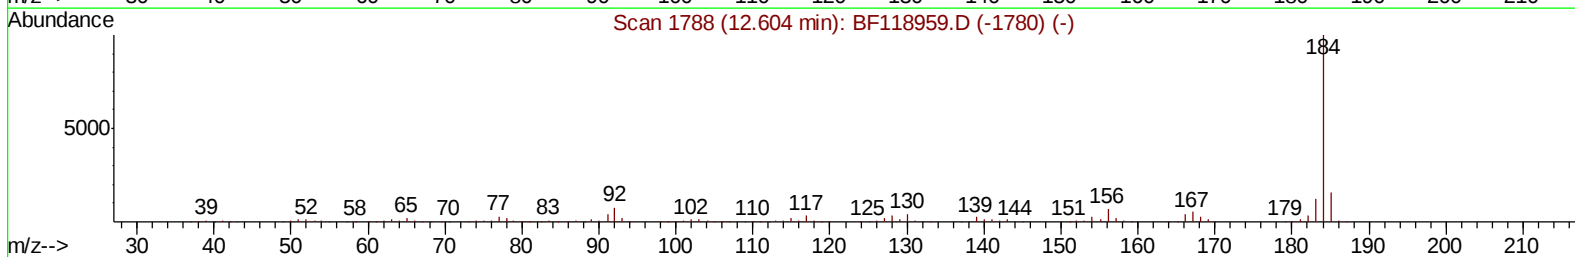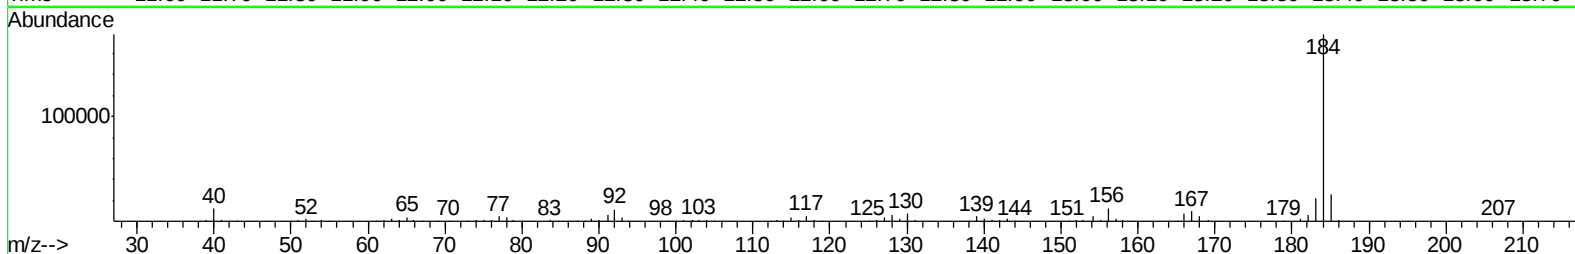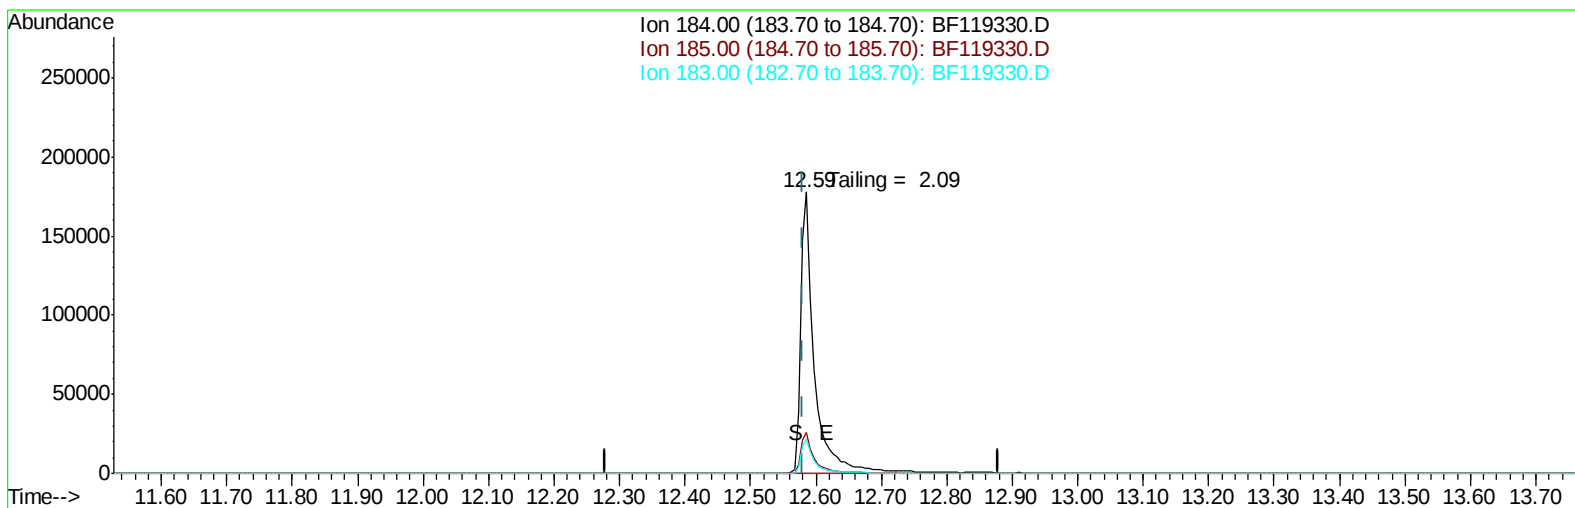

TIC: BF119330.D

(77) Benzidine

12.586min (+0.006) 0.00ng

response 256769

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.44
183.00	12.40	12.40
0.00	0.00	0.00