

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031020\
 Data File : BF119329.D
 Acq On : 10 Mar 2020 21:22
 Operator : CG/JU
 Sample : L1778-25 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S8

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.722	785	788	801	rBV	547410	607636	74.60%	13.811%
2	6.887	813	816	822	rBV	16029	17768	2.18%	0.404%
3	8.004	1003	1006	1018	rBV	797669	752862	92.43%	17.112%
4	9.086	1186	1190	1197	rBV	21362	24248	2.98%	0.551%
5	9.757	1300	1304	1320	rBV	828664	814506	100.00%	18.514%
6	11.245	1553	1557	1565	rBV	757783	724167	88.91%	16.460%
7	12.827	1822	1826	1832	rBV	30600	32176	3.95%	0.731%
8	13.674	1967	1970	1972	rBV	23289	20512	2.52%	0.466%
9	13.745	1977	1982	1983	rBV5	7183	10537	1.29%	0.240%
10	13.886	2002	2006	2015	rBV	776005	763925	93.79%	17.364%
11	14.039	2029	2032	2036	rBV4	19502	25483	3.13%	0.579%
12	15.316	2244	2249	2261	rVB	409989	605692	74.36%	13.767%


Sum of corrected areas: 4399512

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031020\
Data File : BF119329.D
Acq On : 10 Mar 2020 21:22
Operator : CG/JU
Sample : L1778-25 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

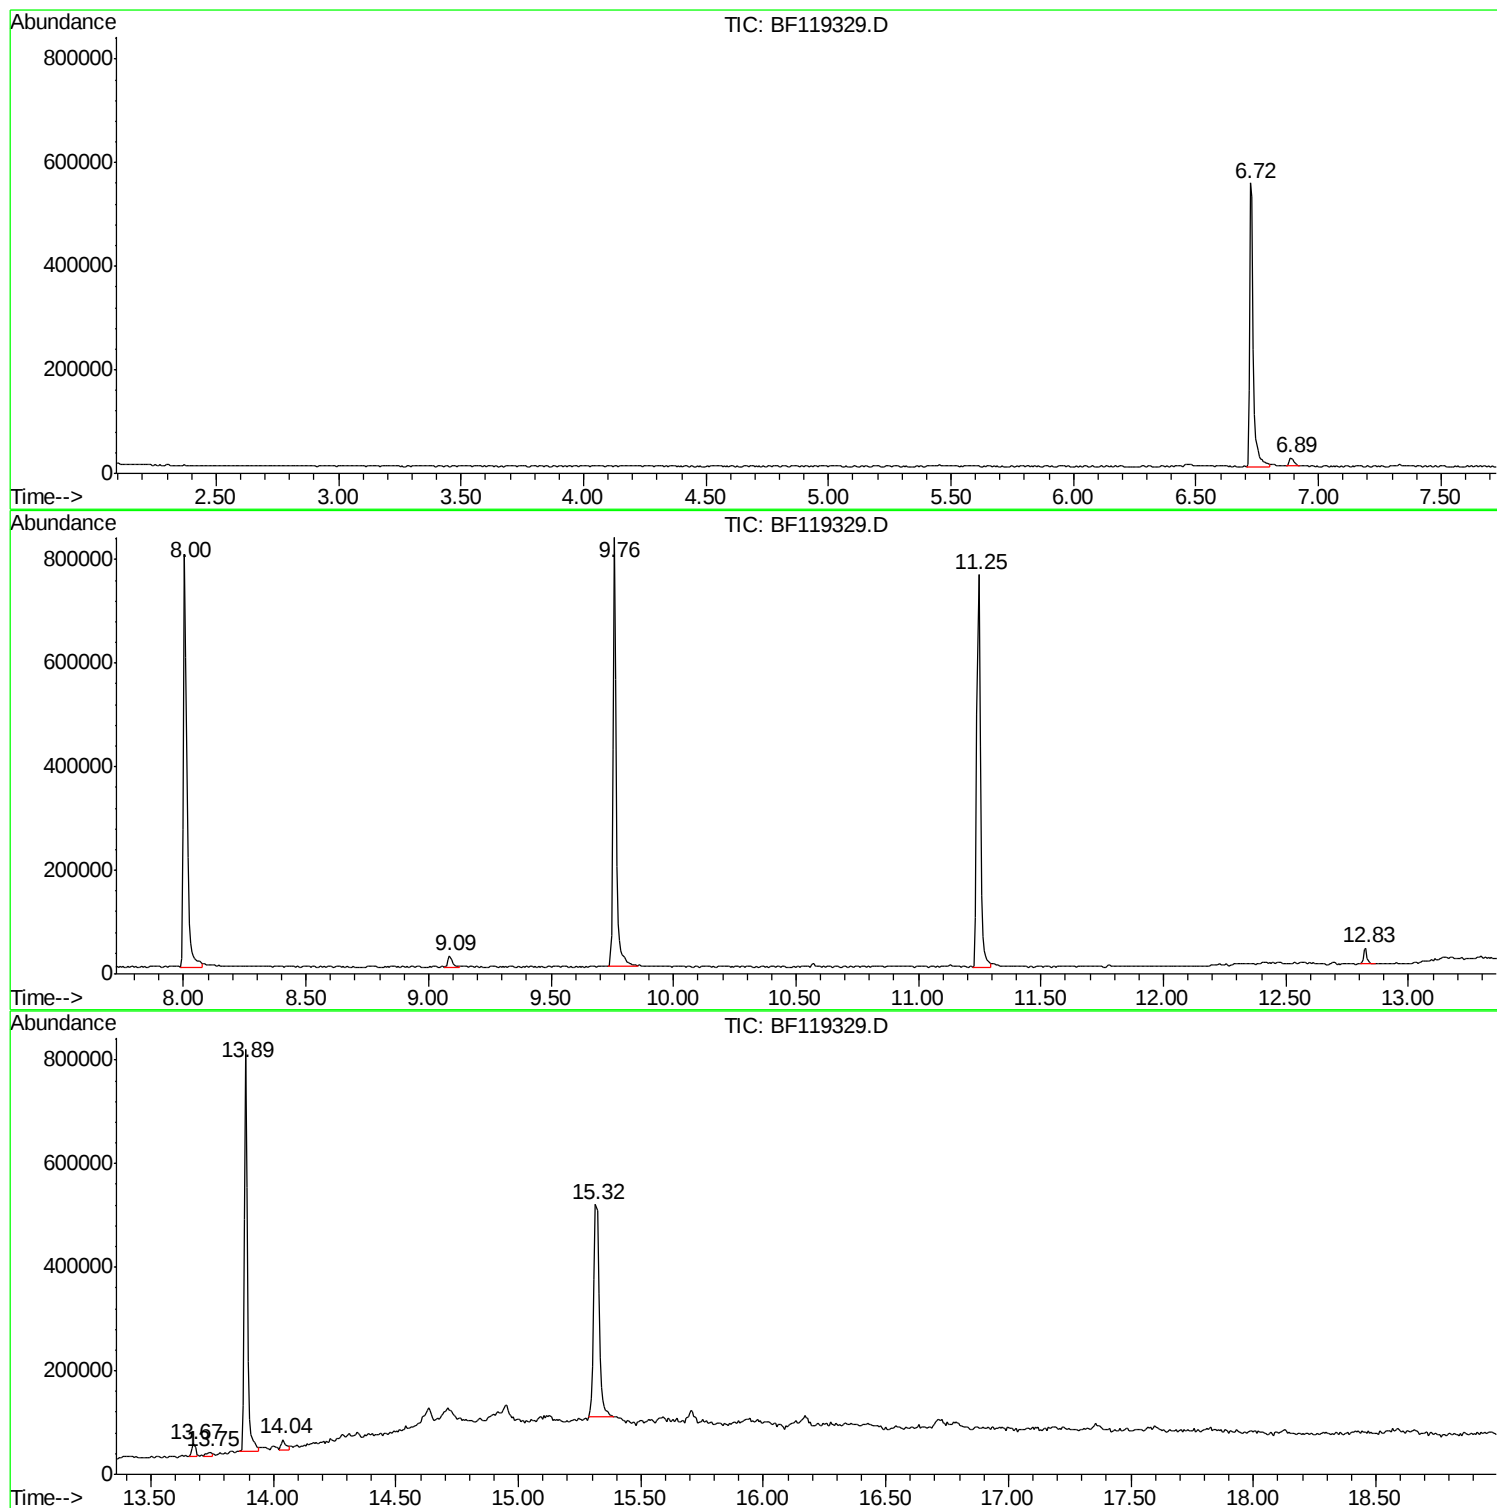

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031020\
Data_File : BF119329.D
Acq_On : 10-Mar-2020 21:222
Operator : CG/JUU
Sample : L1778-25-10XX
Misc :
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
S8

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
