


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031020\
 Data File : BF119311.D
 Acq On : 10 Mar 2020 10:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 06 23:38:46 2020

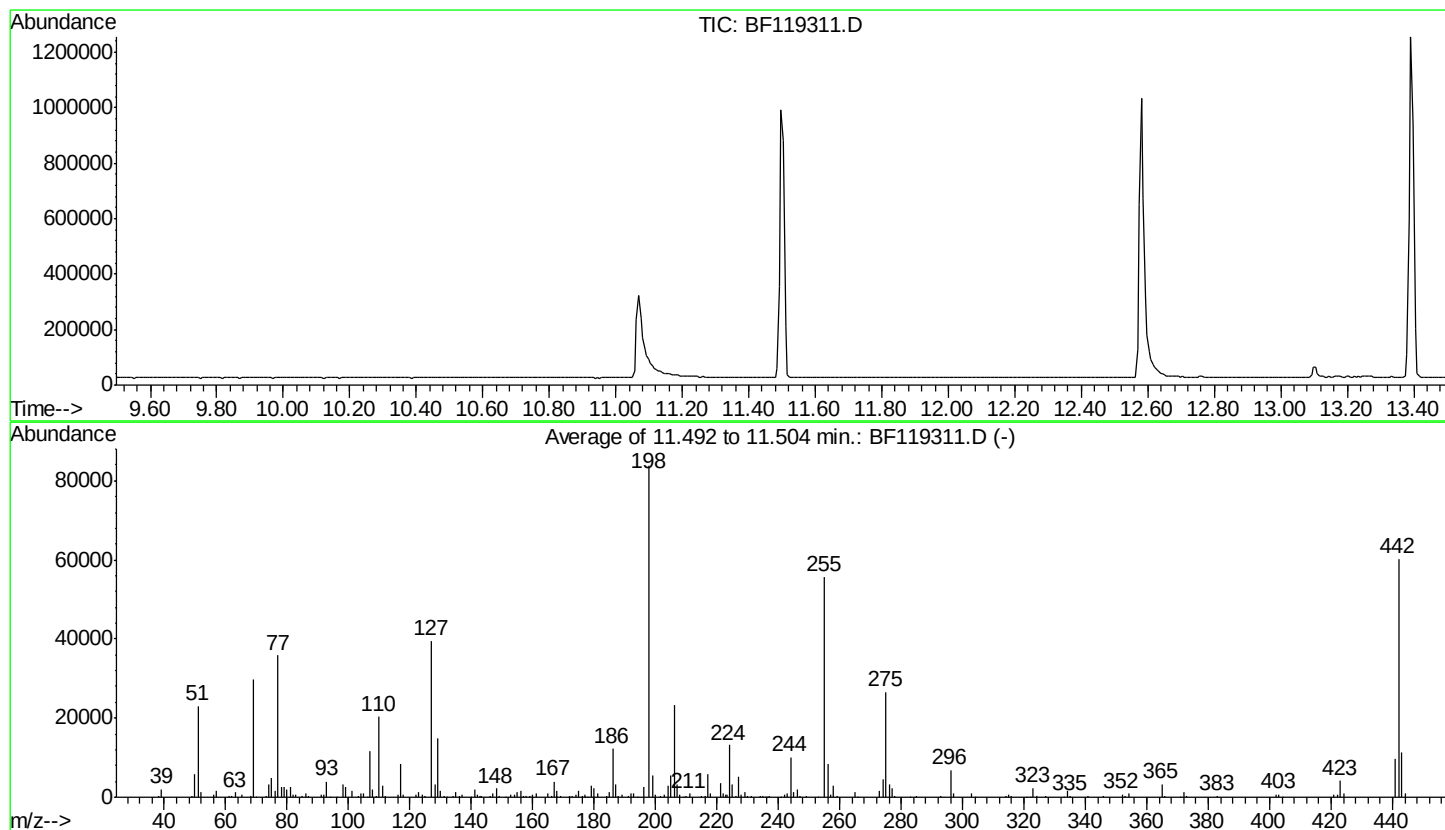

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	23067	PASS
68	69	0.00	2	1.2	372	PASS
69	198	0.00	100	35.5	29786	PASS
70	69	0.00	2	0.4	105	PASS
127	198	10	80	47.3	39632	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83824	PASS
199	198	5	9	6.7	5605	PASS
275	198	10	60	31.8	26680	PASS
365	198	1	100	4.0	3363	PASS
441	198	0.01	100	11.5	9601	PASS
442	198	50	100	71.9	60249	PASS
443	442	15	24	18.9	11408	PASS