

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031022\
 Data File : BF127293.D
 Acq On : 10 Mar 2022 18:29
 Operator : CG\JU
 Sample : PB143220BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143220BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.499	541	546	549	rBV	2481067	2411655	69.00%	12.797%
2	6.504	711	717	720	rBV	2388813	2448361	70.05%	12.992%
3	6.869	775	779	782	rBV	523223	463168	13.25%	2.458%
4	7.434	870	875	878	rBV	1653020	1687784	48.29%	8.956%
5	8.151	992	997	1000	rBV	596164	597520	17.10%	3.171%
6	9.228	1174	1180	1183	rBV	3062116	3017346	86.33%	16.011%
7	9.910	1291	1296	1299	rBV	736859	702718	20.10%	3.729%
8	10.704	1426	1431	1434	rBV	2056213	1918675	54.89%	10.181%
9	11.398	1545	1549	1553	rBV	874516	764686	21.88%	4.058%
10	12.992	1815	1820	1823	rBV	3642685	3495274	100.00%	18.547%
11	14.045	1995	1999	2008	rBV	800356	696032	19.91%	3.693%
12	14.133	2010	2014	2021	rBV	69942	74202	2.12%	0.394%
13	15.533	2247	2252	2260	rBV	467373	568402	16.26%	3.016%




Sum of corrected areas: 18845823

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031022\
Data File : BF127293.D
Acq On : 10 Mar 2022 18:29
Operator : CG\JU
Sample : PB143220BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

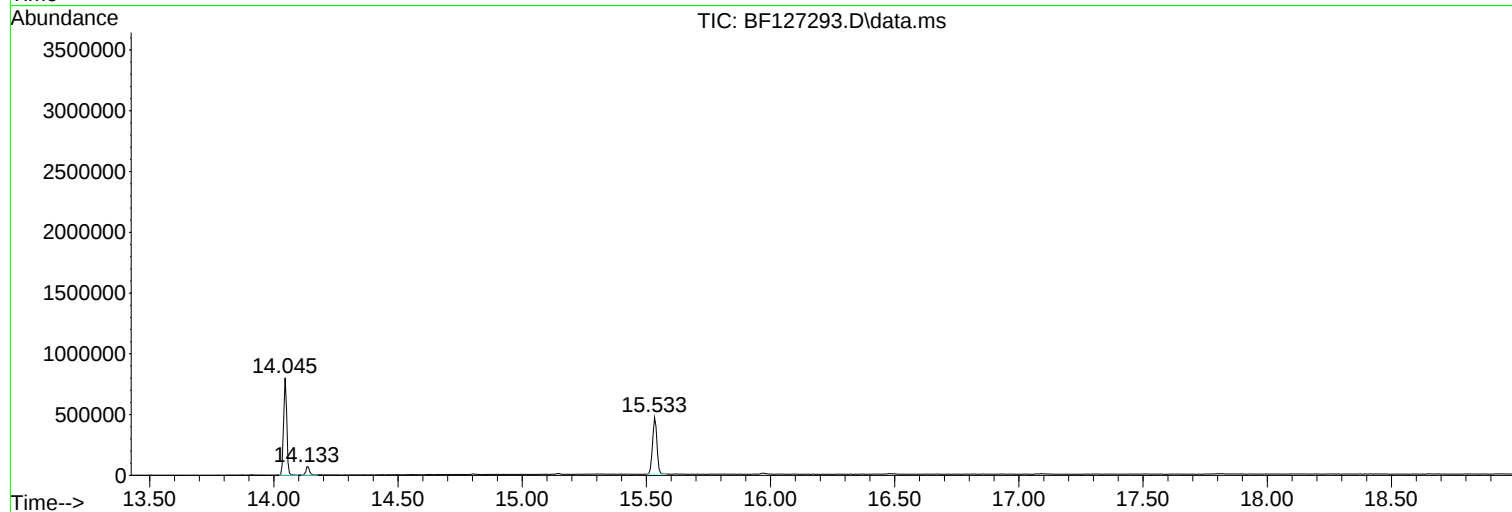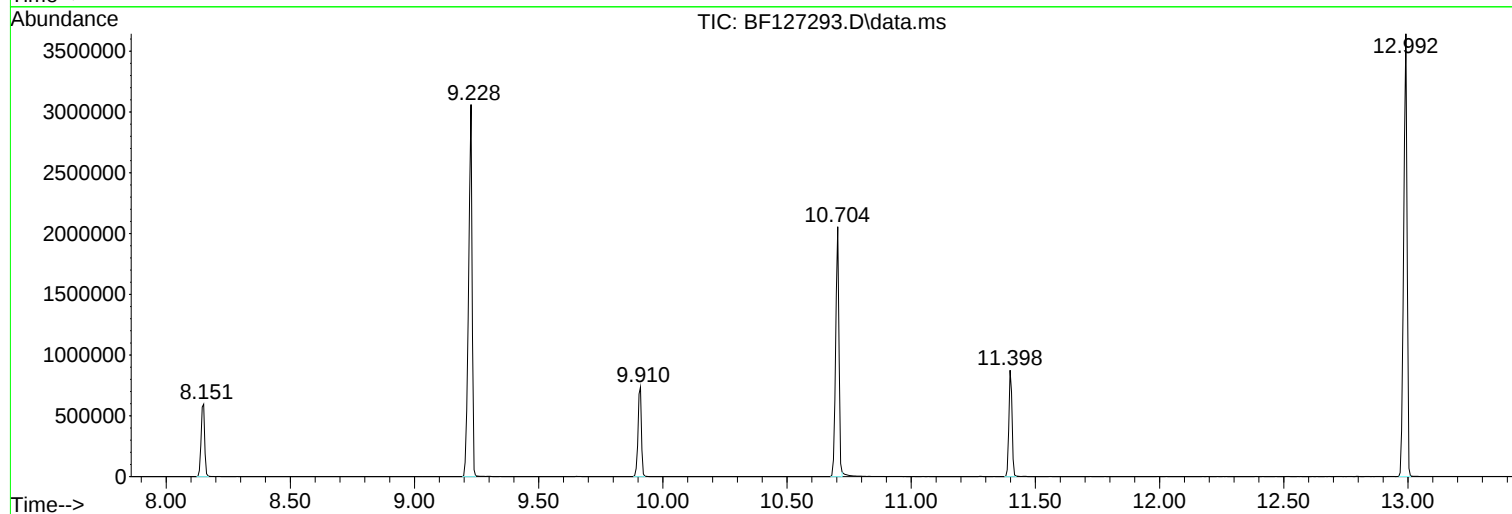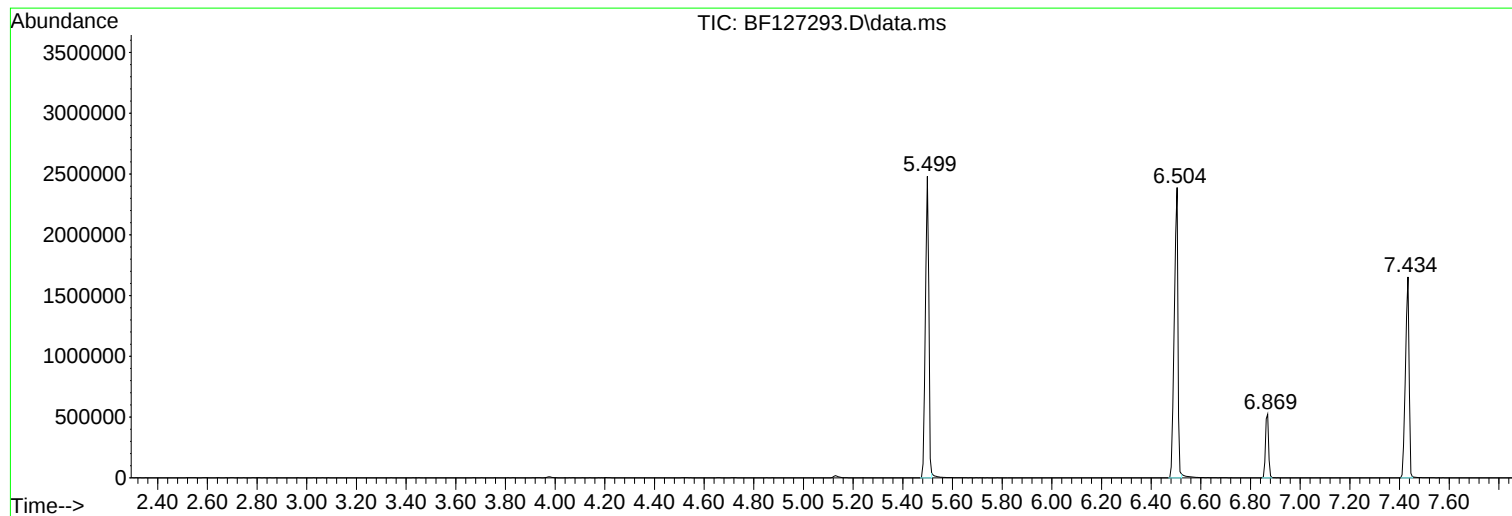

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031022\
Data File : BF127293.D
Acq On : 10 Mar 2022 18:29
Operator : CG\JU
Sample : PB143220BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143220BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.133	2.13 ng	74202	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	49
4			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	43
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	38

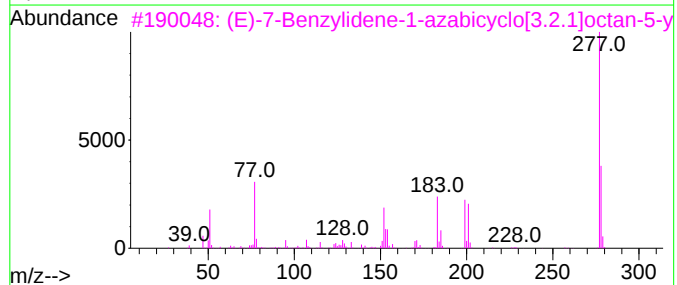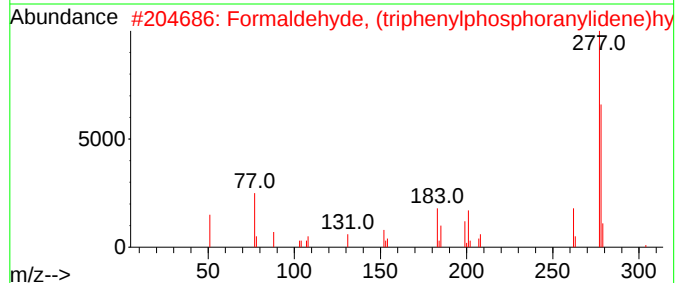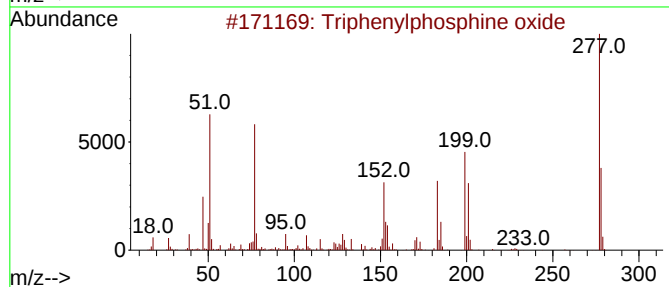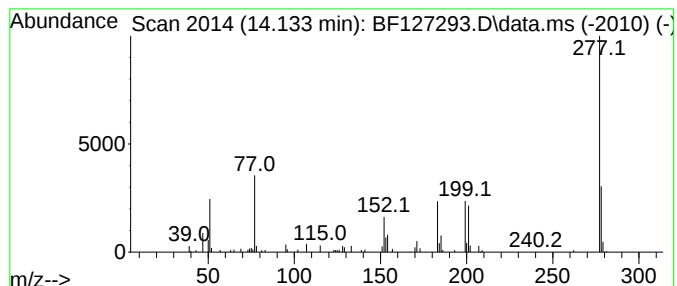

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031022\
Data File : BF127293.D
Acq On : 10 Mar 2022 18:29
Operator : CG\JU
Sample : PB143220BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.133	2.1	ng	74202	5	14.045	696032	20.0