


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031022\
 Data File : BF127283.D
 Acq On : 10 Mar 2022 11:04
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 16:51:53 2022

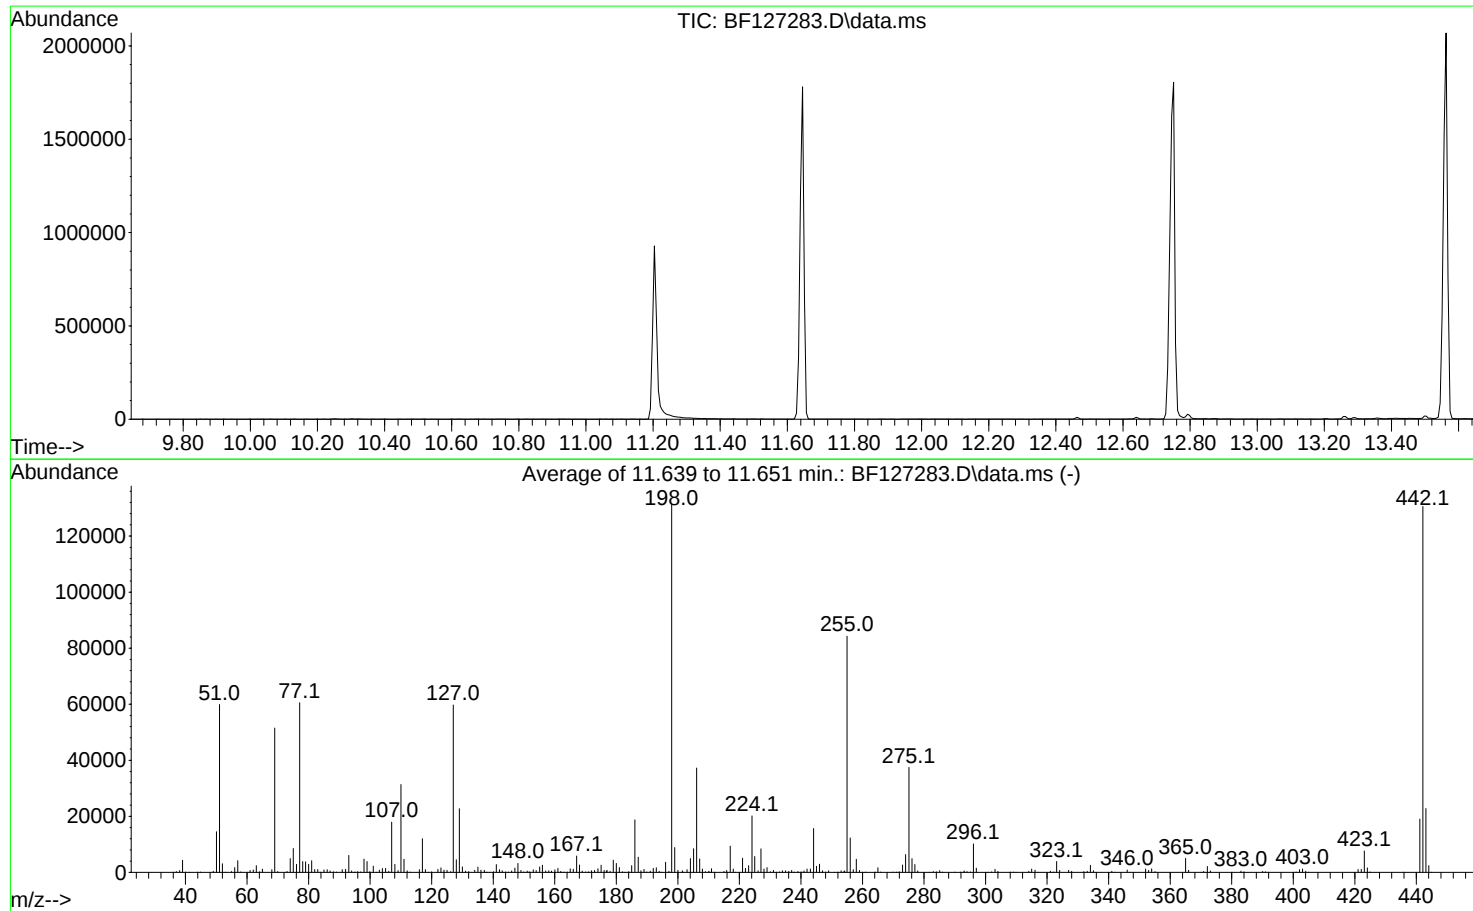

AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	59877	PASS
68	69	0.00	2	1.8	946	PASS
69	198	0.00	100	39.2	51497	PASS
70	69	0.00	2	0.6	294	PASS
127	198	10	80	45.5	59725	PASS
197	198	0.00	2	0.3	419	PASS
198	198	100	100	100.0	131283	PASS
199	198	5	9	6.7	8849	PASS
275	198	10	60	28.5	37459	PASS
365	198	1	100	3.8	4965	PASS
441	198	0.01	100	14.5	19000	PASS
442	442	50	100	100.0	130576	PASS
443	442	15	24	17.4	22765	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/10/2022	BNA_F	<u>BF127283.D</u>
Compound Name	Response	Retention Time
DDT	356287	13.56
DDD	3138	13.26
DDE	126	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3264	359551	0.91

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031022\
Data File : BF127283.D
Acq On : 10 Mar 2022 11:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 10 12:57:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 12:53:35 2022
Response via : Initial Calibration

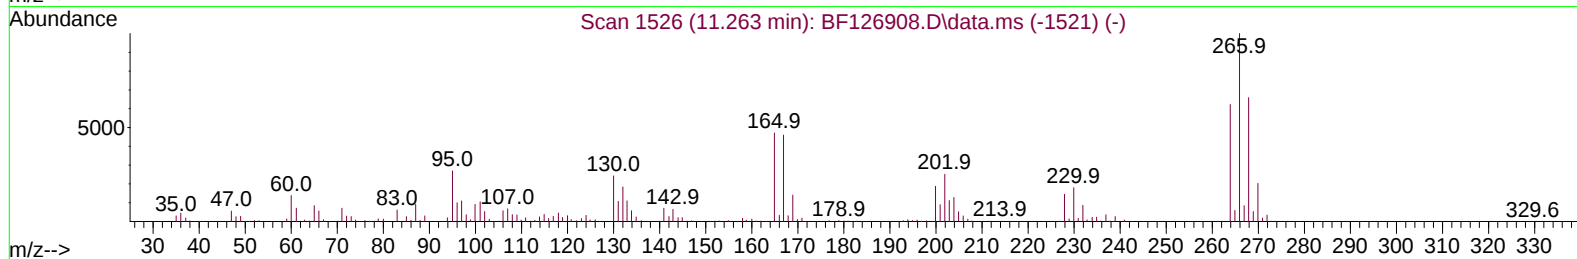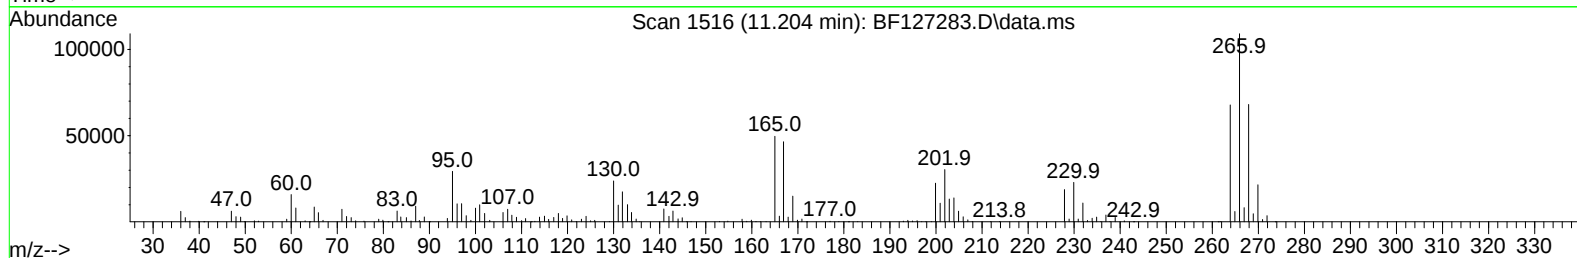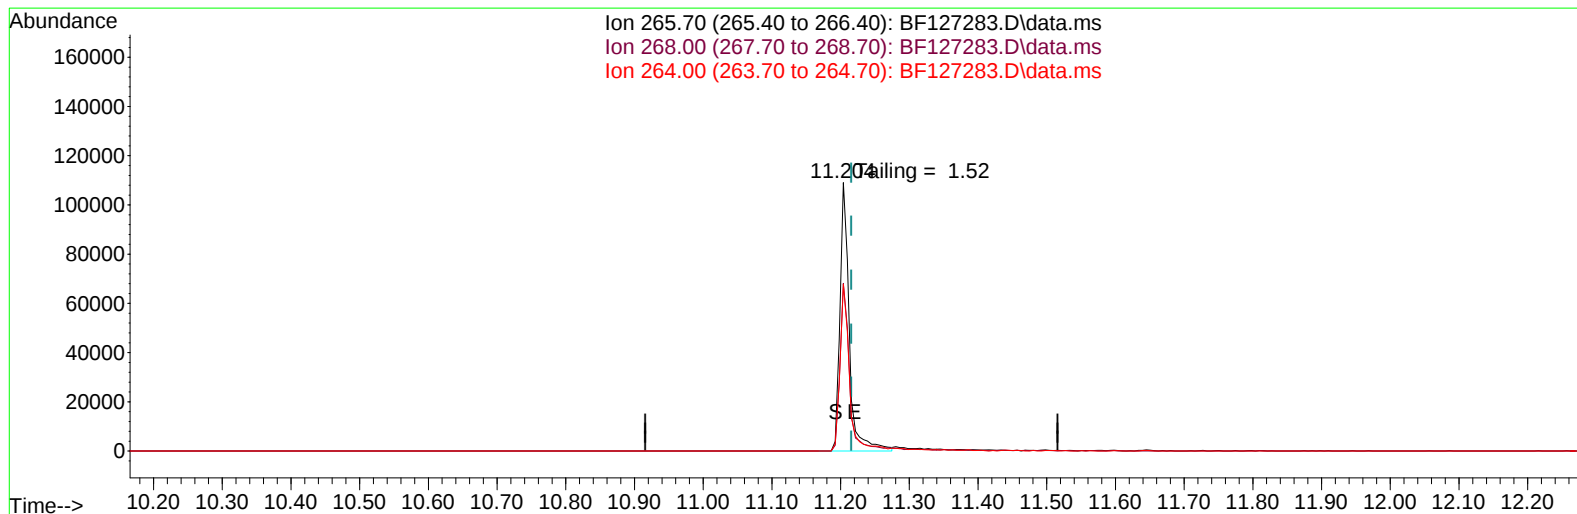

TIC: BF127283.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.012) 22347.76 ng




response 102861

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.46
264.00	63.00	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031022\
 Data File : BF127283.D
 Acq On : 10 Mar 2022 11:04
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 10 12:57:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 10 12:53:35 2022
 Response via : Initial Calibration

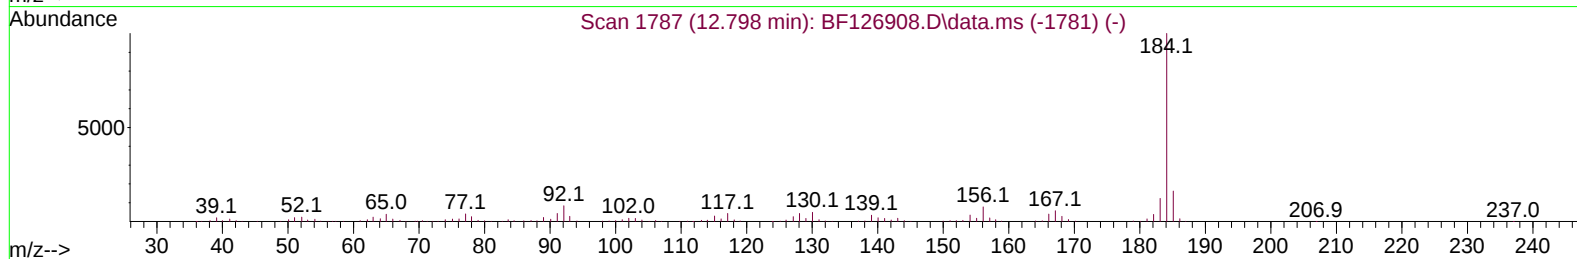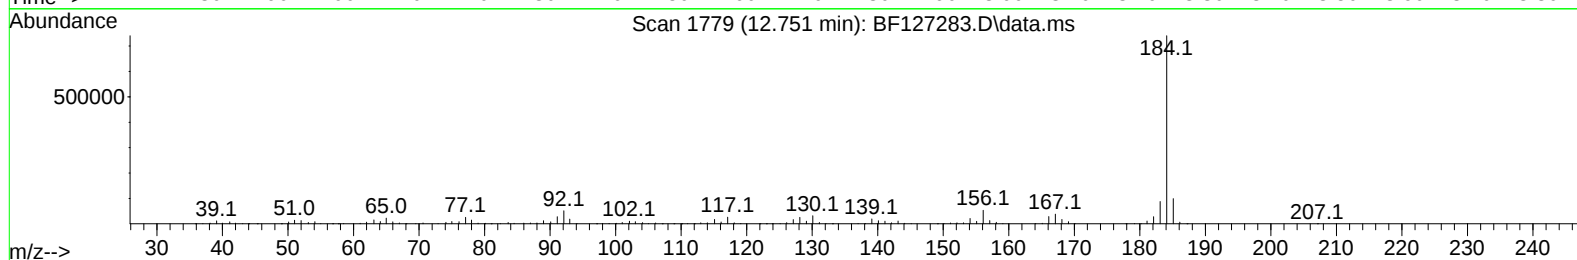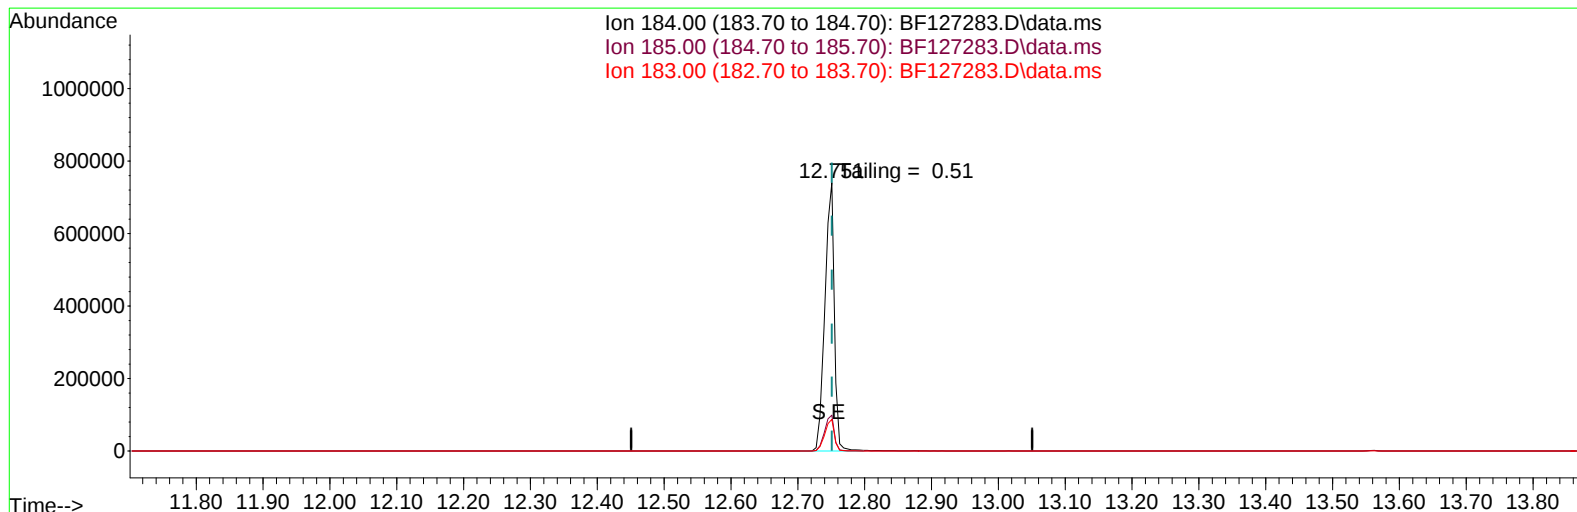

TIC: BF127283.D\data.ms

(77) Benzidine

12.751min (-0.000) 0.00 ng

response 727995

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.34
183.00	10.20	11.82
0.00	0.00	0.00